

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020325\
 Data File : VV038582.D
 Acq On : 03 Feb 2025 13:40
 Operator : SY/MD
 Sample : Q1226-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZP0

Quant Time: Feb 04 07:32:36 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 28 08:06:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	6013	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.784	117	6056	0.500	ug/L	-0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	2907	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	2000	0.330	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	66.000%		
4) 1,2-Dichloroethane-d4	4.969	65	1709	0.353	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	70.000%		
7) 1,2-Dichloropropane-d6	5.995	67	2013	0.338	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	68.000%		
8) Toluene-d8	7.253	98	3743	0.314	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	62.000%#		
10) 1,1,2,2-Tetrachloroeth...	10.145	84	1833	0.361	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	72.000%		
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.280	62	170	0.022	ug/L #	7
6) Trichloroethene	5.828	95	8720	1.743	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020325\
Data File : VV038582.D
Acq On : 03 Feb 2025 13:40
Operator : SY/MD
Sample : Q1226-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCZP0

Quant Time: Feb 04 07:32:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 28 08:06:10 2025
Response via : Initial Calibration




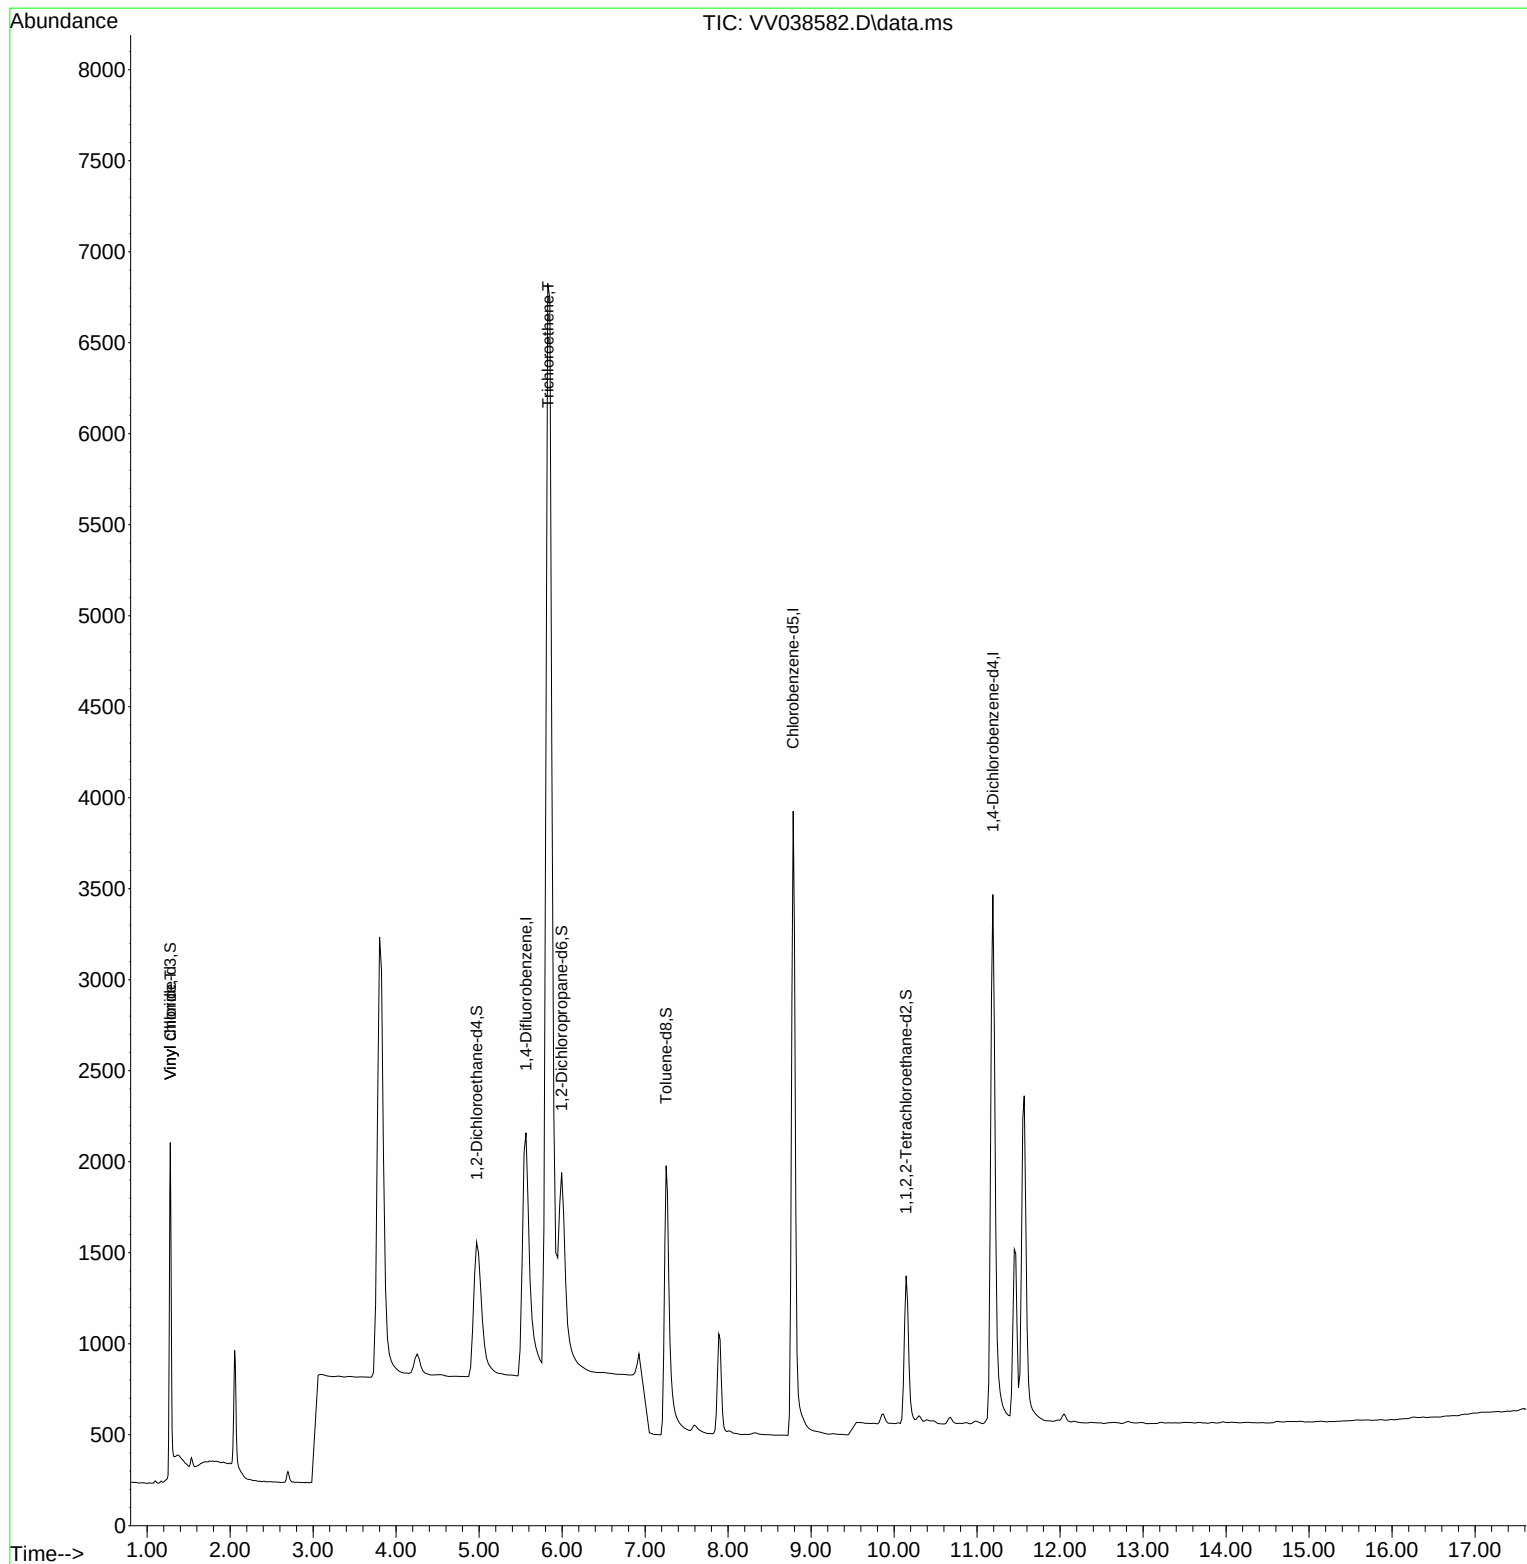


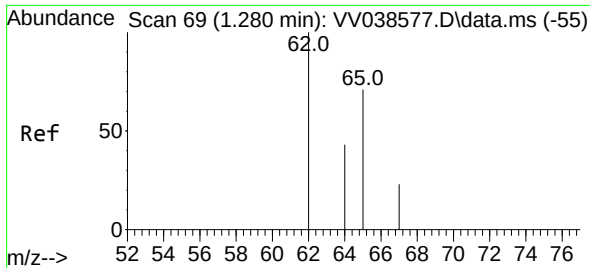

#3
 Vinyl chloride
 Concen: 0.022 ug/L
 RT: 1.280 min Scan# 69
 Delta R.T. -0.000 min
 Lab File: VV038582.D
 Acq: 03 Feb 2025 13:40

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZP0

Tgt Ion: 62 Resp: 170
 Ion Ratio Lower Upper
 62 100
 64 88.8 24.4 45.2#

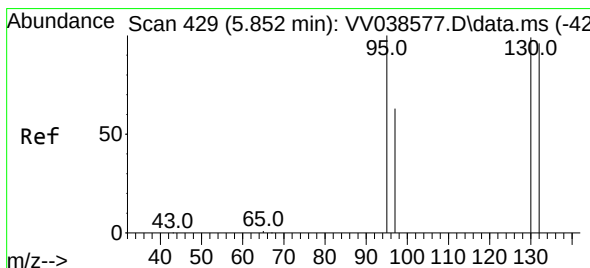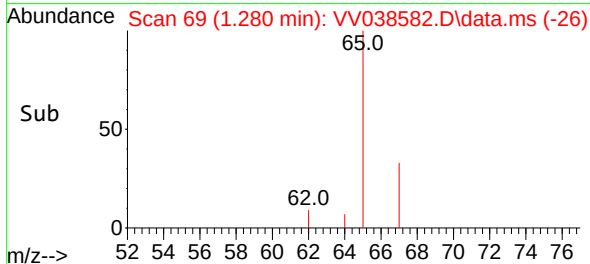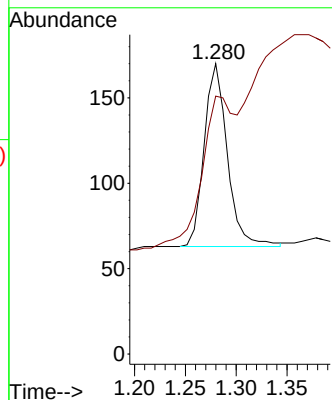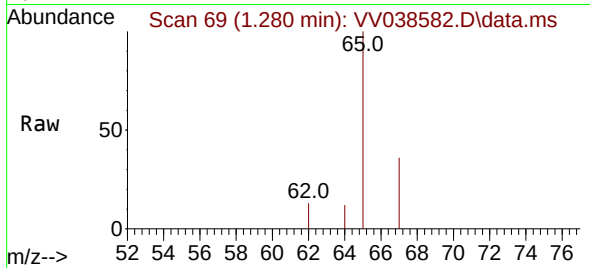

#6
 Trichloroethene
 Concen: 1.743 ug/L
 RT: 5.828 min Scan# 428
 Delta R.T. -0.024 min
 Lab File: VV038582.D
 Acq: 03 Feb 2025 13:40

Tgt Ion: 95 Resp: 8720
 Ion Ratio Lower Upper
 95 100
 97 64.5 47.9 88.9
 132 87.5 68.2 126.6
 130 96.0 69.7 129.5

