

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020325\
 Data File : VV038588.D
 Acq On : 03 Feb 2025 16:05
 Operator : SY/MD
 Sample : Q1226-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZP2

Quant Time: Feb 04 07:33:40 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 28 08:06:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	5433	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	5521	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	2663	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	2091	0.382	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	76.000%		
4) 1,2-Dichloroethane-d4	4.969	65	1980	0.453	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	90.000%		
7) 1,2-Dichloropropane-d6	5.995	67	2275	0.419	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	84.000%		
8) Toluene-d8	7.253	98	4249	0.391	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	78.000%		
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2271	0.491	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	98.000%		
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.280	62	325	0.046	ug/L #	64
6) Trichloroethene	5.828	95	5632	1.235	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020325\
Data File : VV038588.D
Acq On : 03 Feb 2025 16:05
Operator : SY/MD
Sample : Q1226-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCZP2

Quant Time: Feb 04 07:33:40 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 28 08:06:10 2025
Response via : Initial Calibration

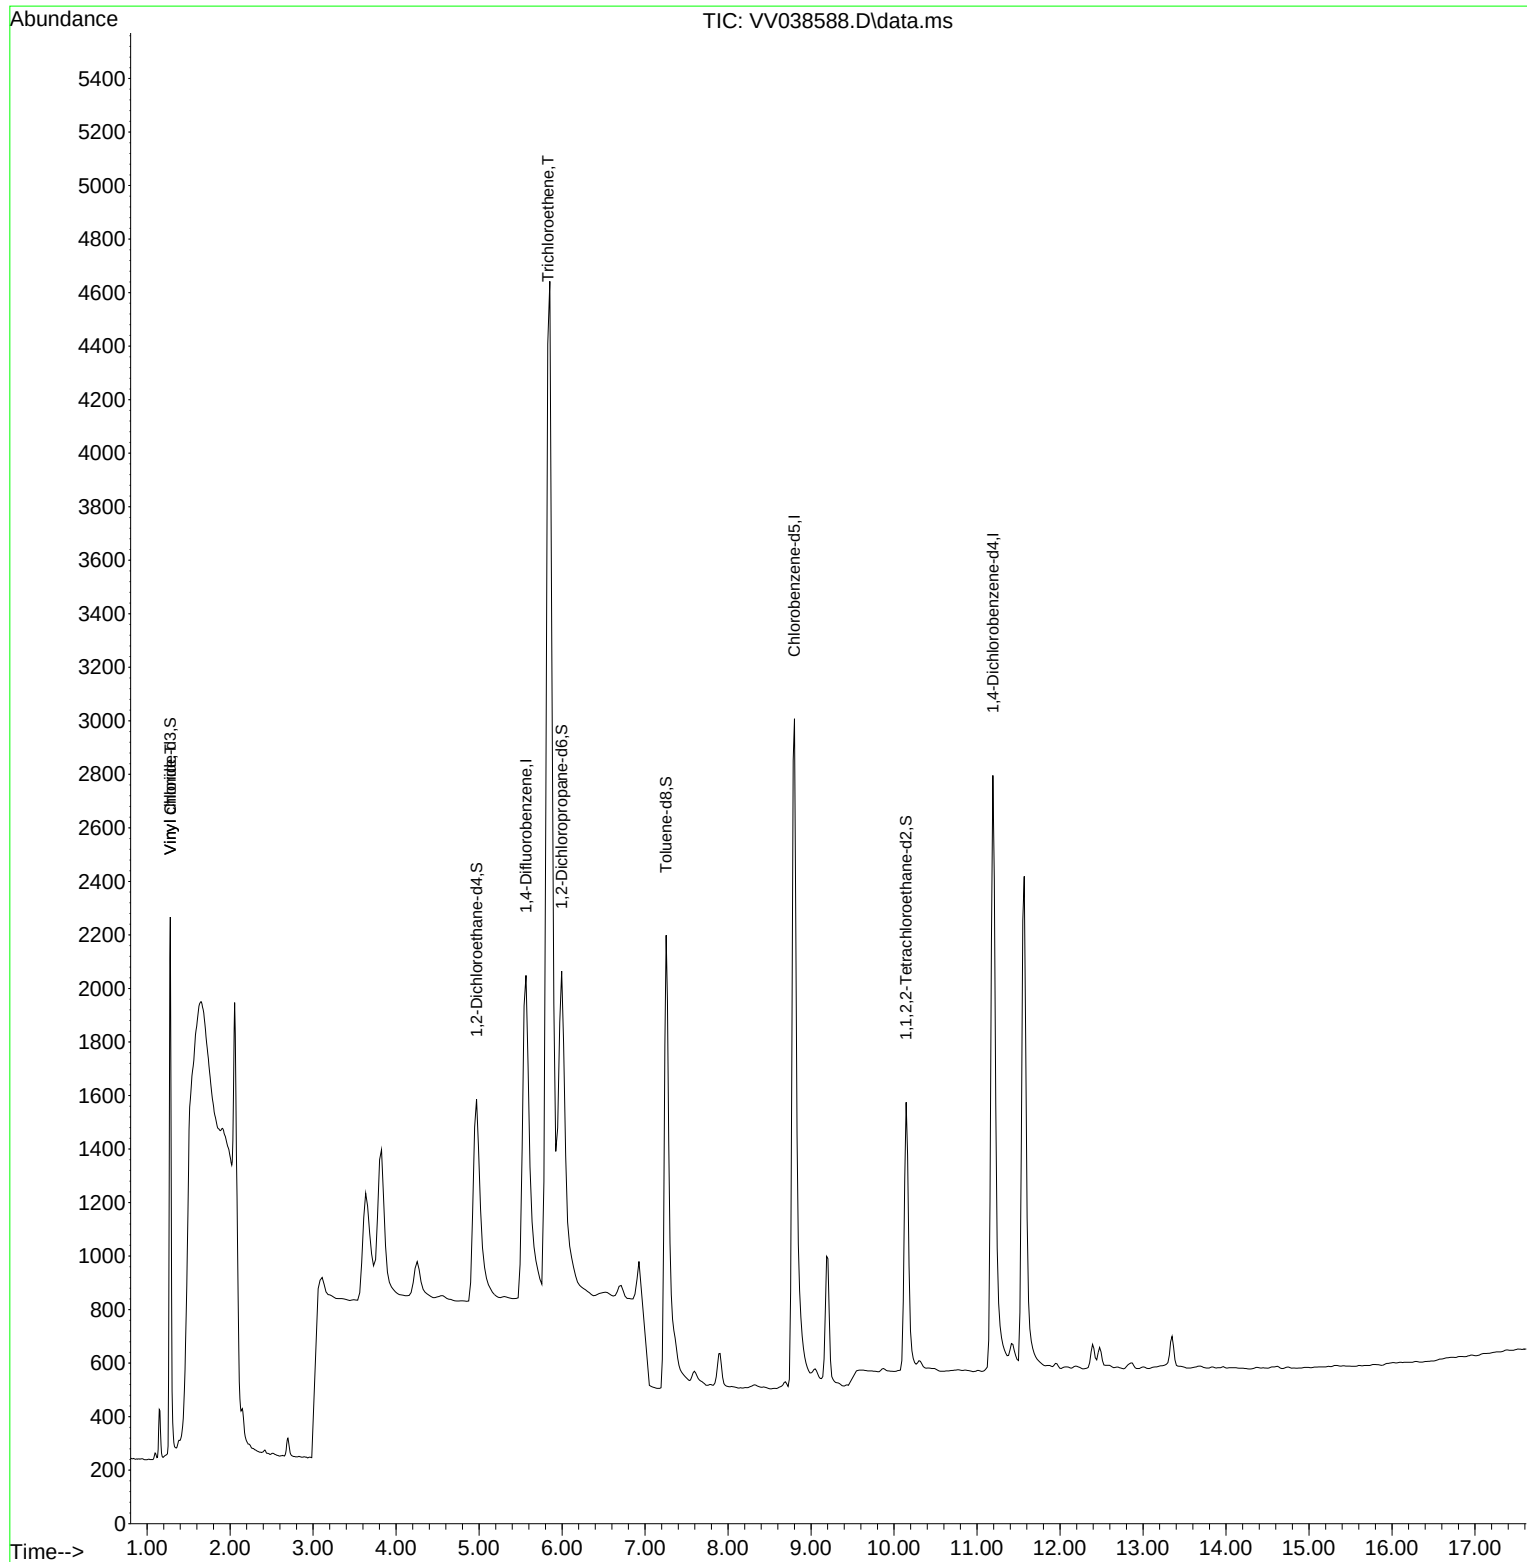

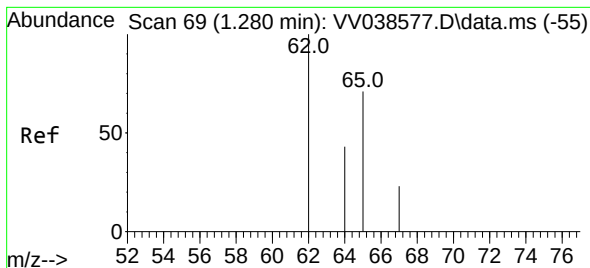

#3

Vinyl chloride

Concen: 0.046 ug/L

RT: 1.280 min Scan# 69

Delta R.T. 0.000 min

Lab File: VV038588.D

Acq: 03 Feb 2025 16:05

Instrument :

MSVOA_V

ClientSampleId :





DCZP2

Tgt Ion: 62 Resp: 325

Ion Ratio Lower Upper

62 100

64 55.4 24.4 45.2#

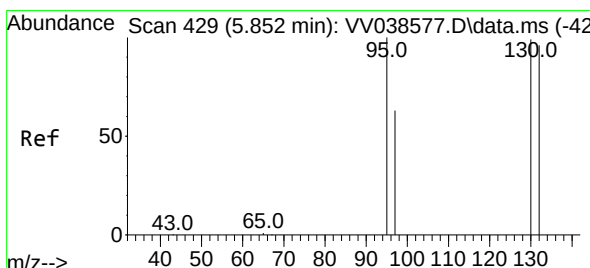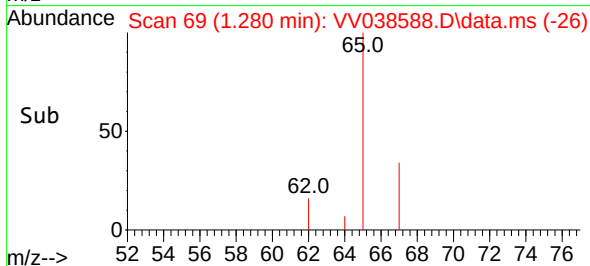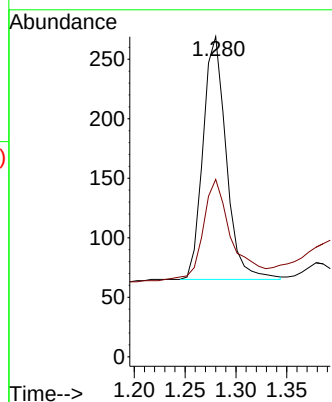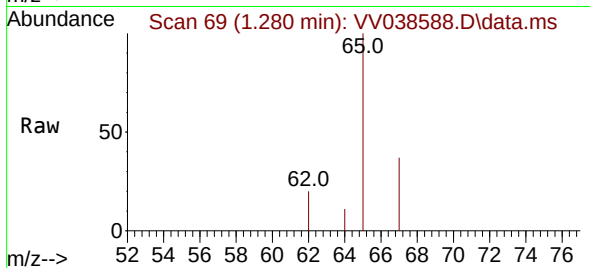

#6

Trichloroethene

Concen: 1.235 ug/L

RT: 5.828 min Scan# 428

Delta R.T. -0.024 min

Lab File: VV038588.D

Acq: 03 Feb 2025 16:05

Tgt Ion: 95 Resp: 5632

Ion Ratio Lower Upper

95 100

97 64.5 47.9 88.9

132 82.7 68.2 126.6

130 90.9 69.7 129.5

