

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020325\
 Data File : VV038591.D
 Acq On : 03 Feb 2025 17:18
 Operator : SY/MD
 Sample : Q1226-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZK6

Quant Time: Feb 04 07:34:11 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 28 08:06:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	4455	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	4621	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	2139	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	1565	0.348	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	70.000%		
4) 1,2-Dichloroethane-d4	4.970	65	1576	0.439	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	88.000%		
7) 1,2-Dichloropropane-d6	5.996	67	1722	0.379	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	76.000%		
8) Toluene-d8	7.254	98	2991	0.329	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	66.000%#		
10) 1,1,2,2-Tetrachloroeth...	10.146	84	1964	0.507	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	102.000%		
Target Compounds						
6) Trichloroethene	5.852	95	342	0.090	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020325\
Data File : VV038591.D
Acq On : 03 Feb 2025 17:18
Operator : SY/MD
Sample : Q1226-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCZK6


Quant Time: Feb 04 07:34:11 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 28 08:06:10 2025
Response via : Initial Calibration

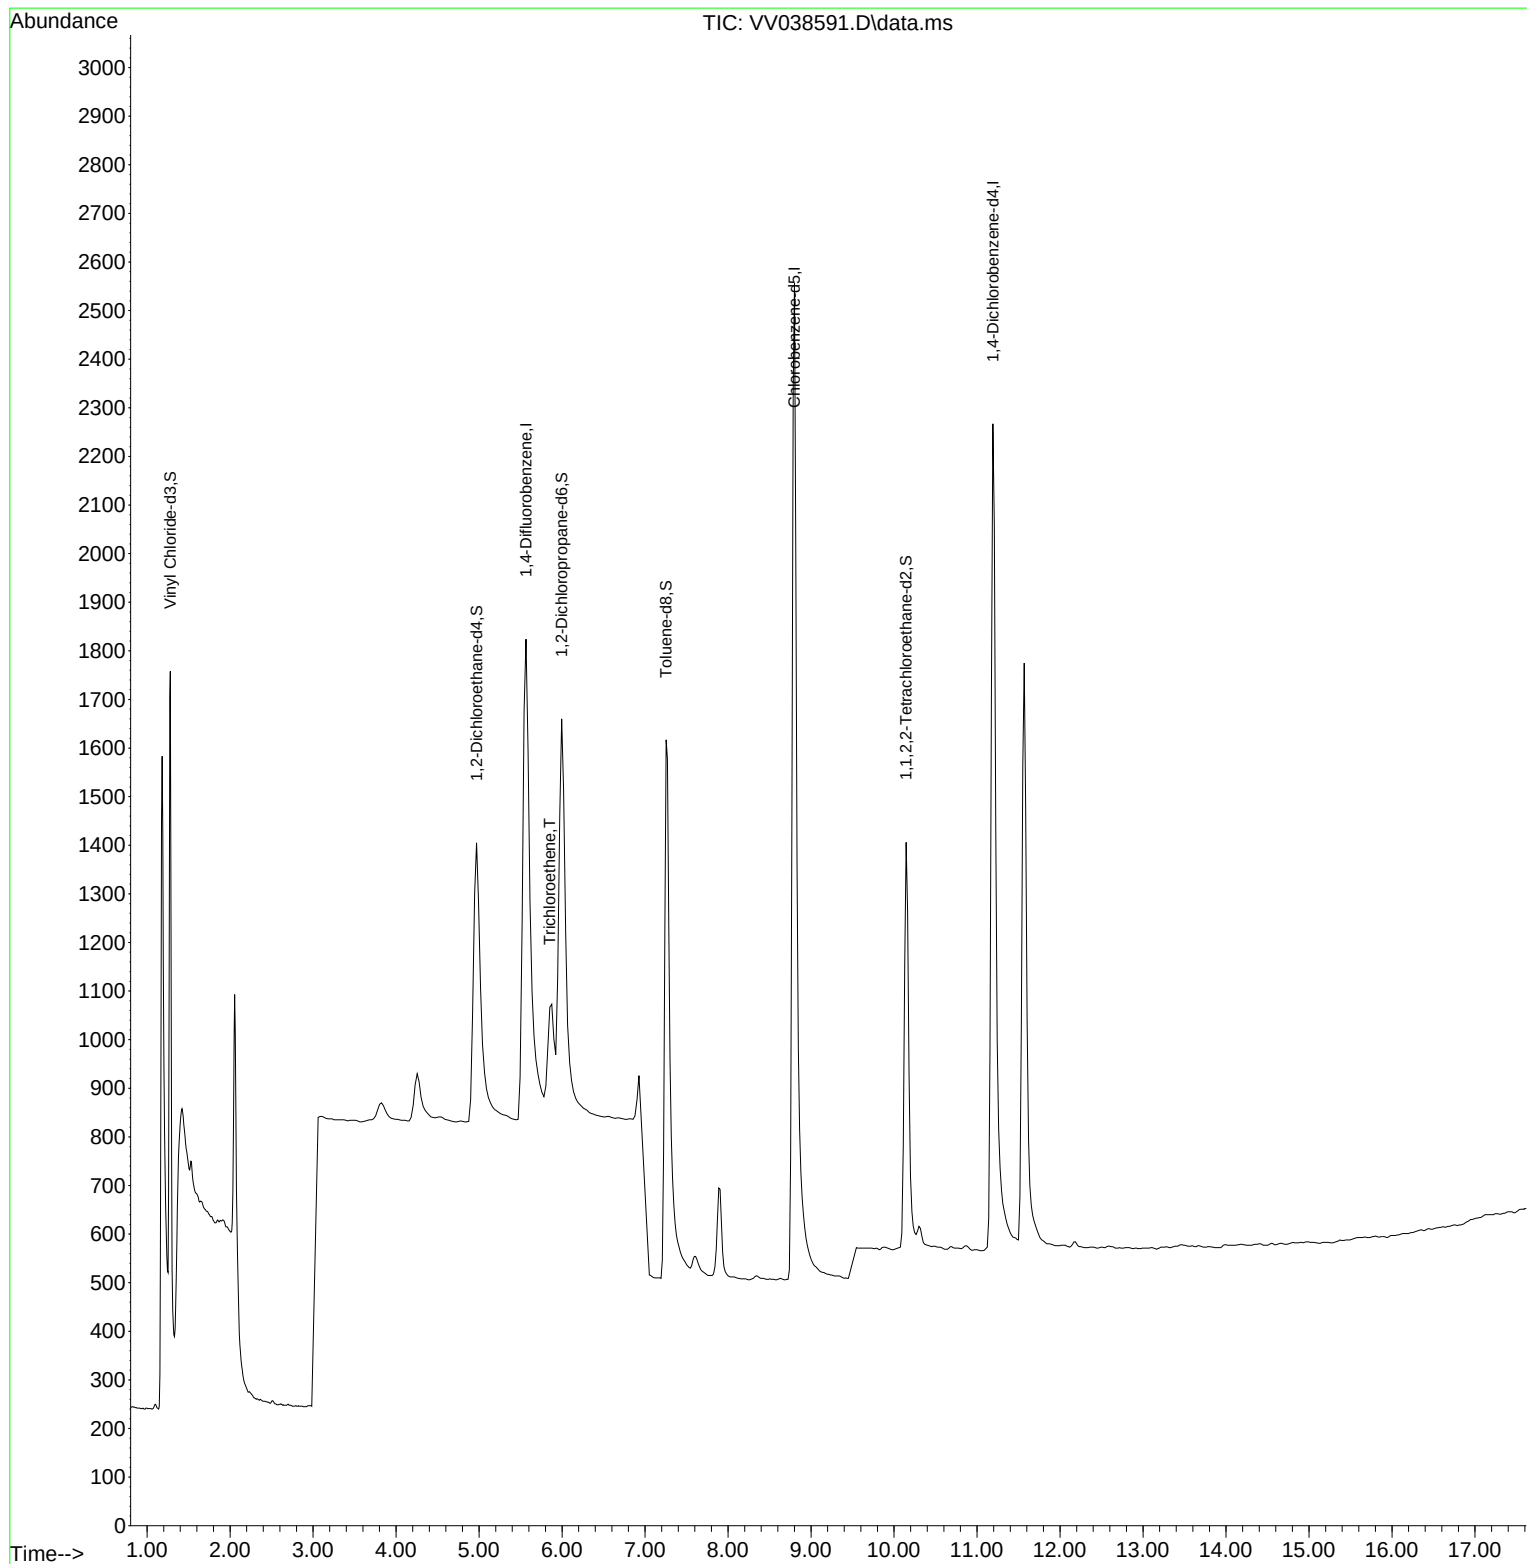

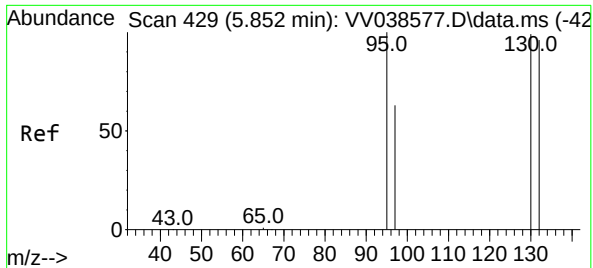

#6
 Trichloroethene
 Concen: 0.090 ug/L
 RT: 5.852 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: VV038591.D
 Acq: 03 Feb 2025 17:18

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZK6

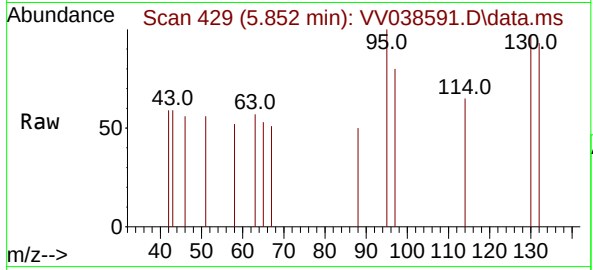

Tgt Ion: 95 Resp: 342

Ion	Ratio	Lower	Upper
95	100		
97	80.0	47.9	88.9
132	93.0	68.2	126.6
130	96.5	69.7	129.5

