

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020325\
 Data File : VV038593.D
 Acq On : 03 Feb 2025 18:07
 Operator : SY/MD
 Sample : Q1226-22
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZL9

Quant Time: Feb 04 07:34:32 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 28 08:06:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	8796	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	8556	0.500	ug/L	-0.02
11) 1,4-Dichlorobenzene-d4	11.174	152	4717	0.500	ug/L	#-0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	3207	0.362	ug/L	0.00
Spiked Amount 0.500	Range	40 - 130	Recovery	=	72.000%	
4) 1,2-Dichloroethane-d4	4.969	65	2740	0.387	ug/L	0.00
Spiked Amount 0.500	Range	70 - 130	Recovery	=	78.000%	
7) 1,2-Dichloropropane-d6	5.995	67	3167	0.377	ug/L	0.00
Spiked Amount 0.500	Range	60 - 140	Recovery	=	76.000%	
8) Toluene-d8	7.253	98	6568	0.390	ug/L	0.00
Spiked Amount 0.500	Range	70 - 130	Recovery	=	78.000%	
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2888	0.403	ug/L	0.00
Spiked Amount 0.500	Range	65 - 120	Recovery	=	80.000%	
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.280	62	6336	0.554	ug/L	83
6) Trichloroethene	5.828	95	95585	13.525	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020325\
Data File : VV038593.D
Acq On : 03 Feb 2025 18:07
Operator : SY/MD
Sample : Q1226-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCZL9

Quant Time: Feb 04 07:34:32 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 28 08:06:10 2025
Response via : Initial Calibration

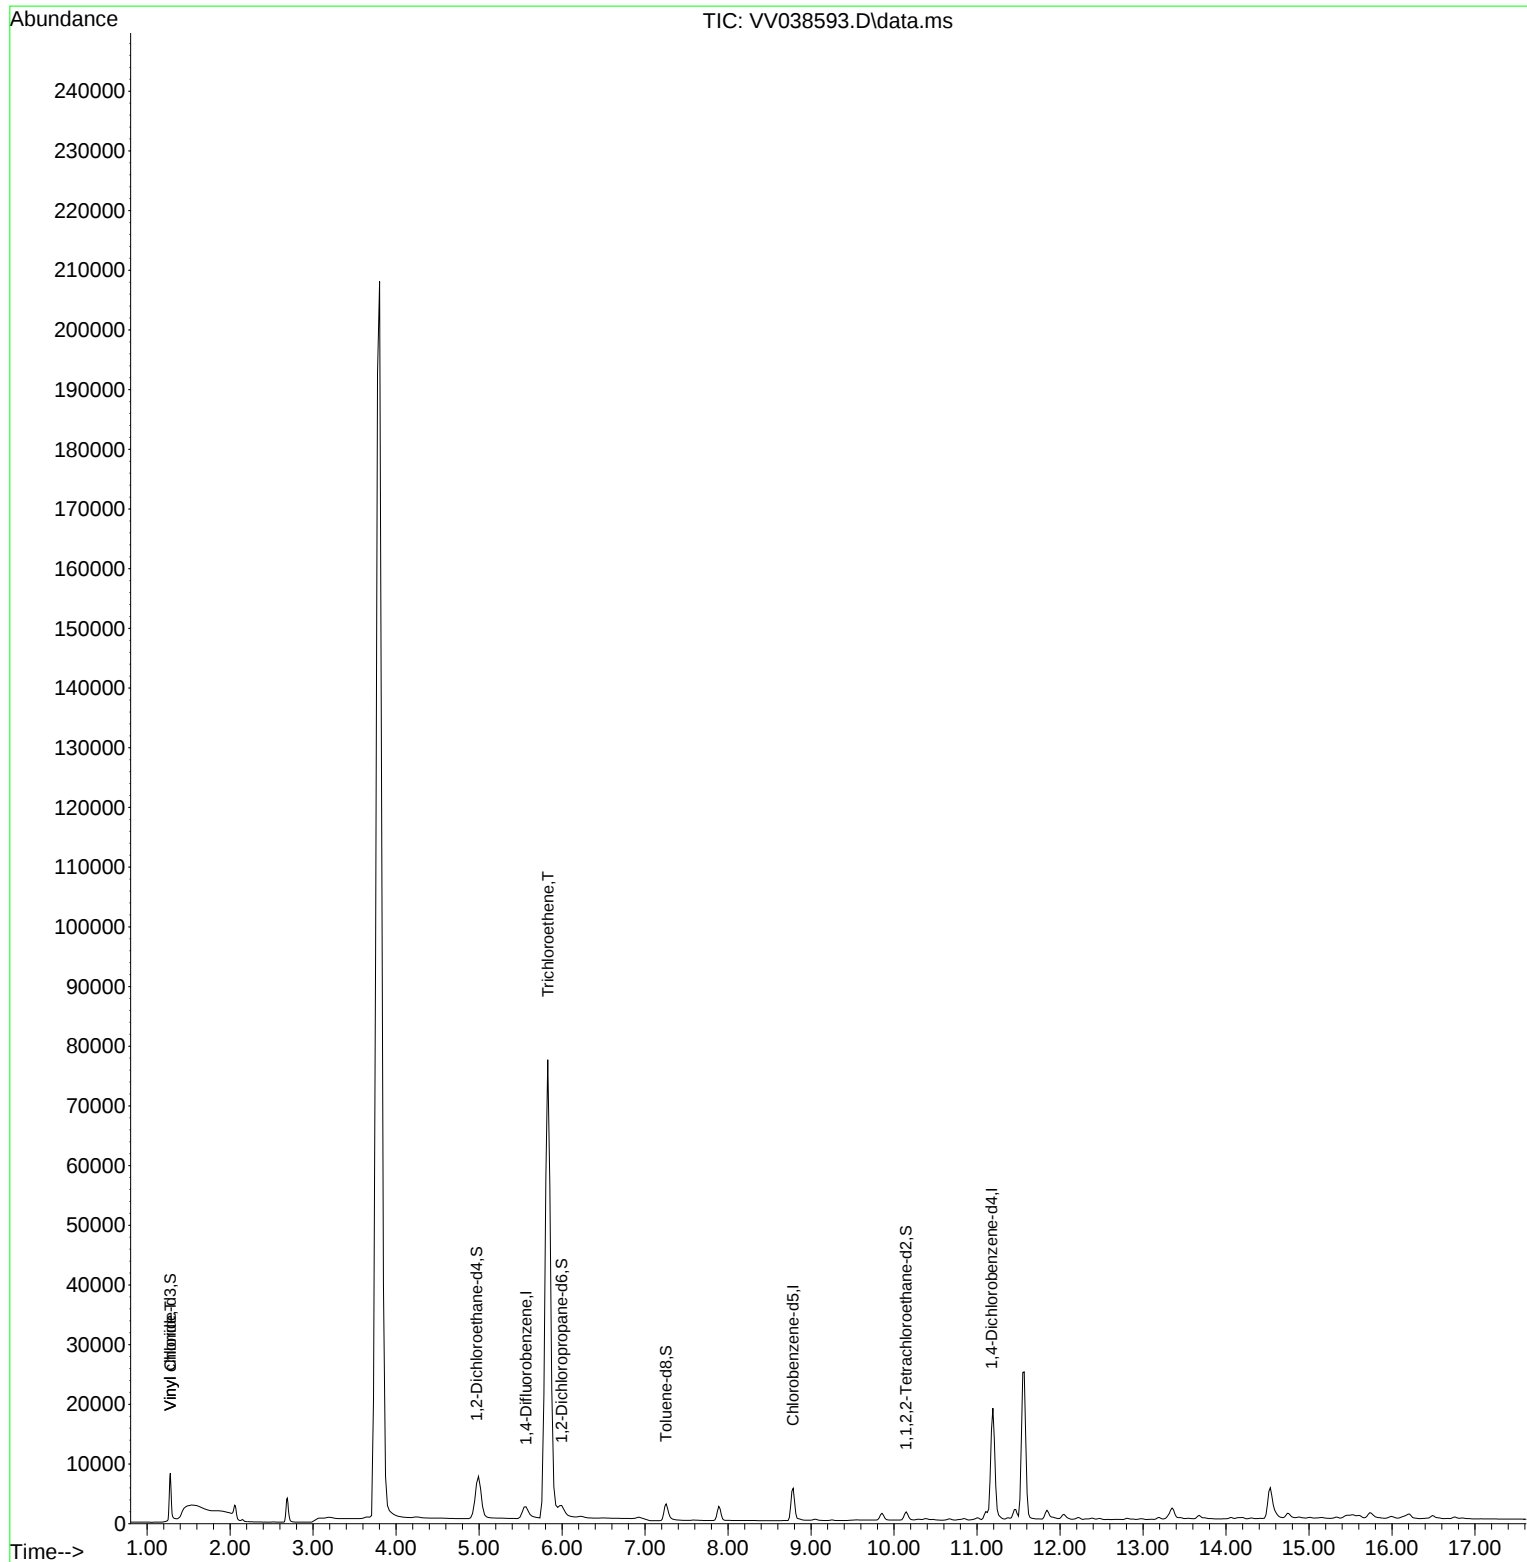

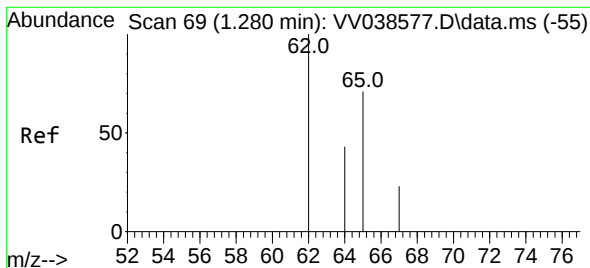

#3

Vinyl chloride

Concen: 0.554 ug/L

RT: 1.280 min Scan# 61

Delta R.T. 0.000 min

Lab File: VV038593.D

Acq: 03 Feb 2025 18:07

Instrument :

MSVOA_V

ClientSampleId :





DCZL9

Tgt Ion: 62 Resp: 6336

Ion Ratio Lower Upper

62 100

64 44.4 24.4 45.2

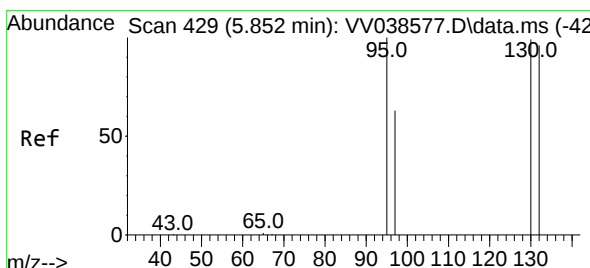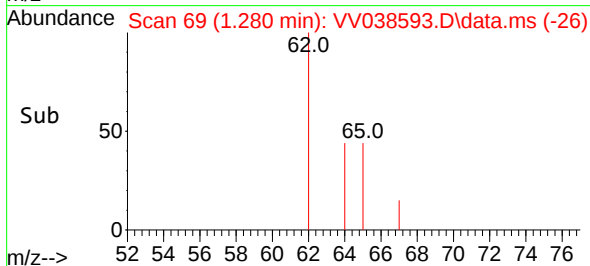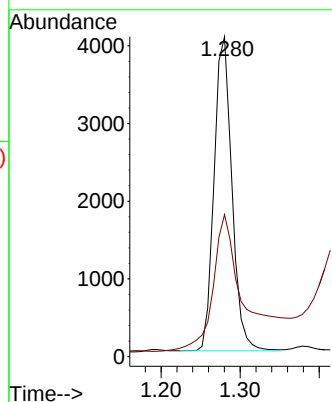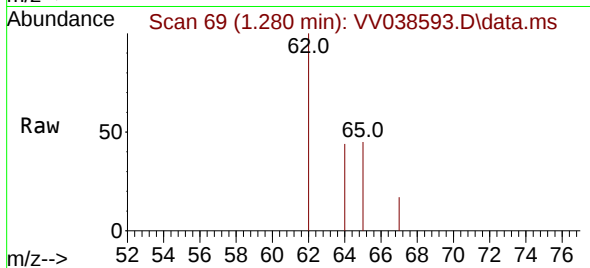

#6

Trichloroethene

Concen: 13.525 ug/L

RT: 5.828 min Scan# 428

Delta R.T. -0.024 min

Lab File: VV038593.D

Acq: 03 Feb 2025 18:07

Tgt Ion: 95 Resp: 95585

Ion Ratio Lower Upper

95 100

97 65.9 47.9 88.9

132 104.0 68.2 126.6

130 105.5 69.7 129.5

