

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020325\
 Data File : VV038595.D
 Acq On : 03 Feb 2025 18:55
 Operator : SY/MD
 Sample : Q1226-24
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZN2

Quant Time: Feb 04 07:34:53 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 28 08:06:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	7930	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	7919	0.500	ug/L	-0.01
11) 1,4-Dichlorobenzene-d4	11.192	152	3678	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.274	65	3052	0.382	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	76.000%		
4) 1,2-Dichloroethane-d4	4.970	65	2623	0.411	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	82.000%		
7) 1,2-Dichloropropane-d6	5.996	67	3210	0.412	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	82.000%		
8) Toluene-d8	7.254	98	6330	0.406	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	82.000%		
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2888	0.435	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	88.000%		
Target Compounds						Qvalue
6) Trichloroethene	5.853	95	2617	0.400	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020325\
Data File : VV038595.D
Acq On : 03 Feb 2025 18:55
Operator : SY/MD
Sample : Q1226-24
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCZN2


Quant Time: Feb 04 07:34:53 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 28 08:06:10 2025
Response via : Initial Calibration

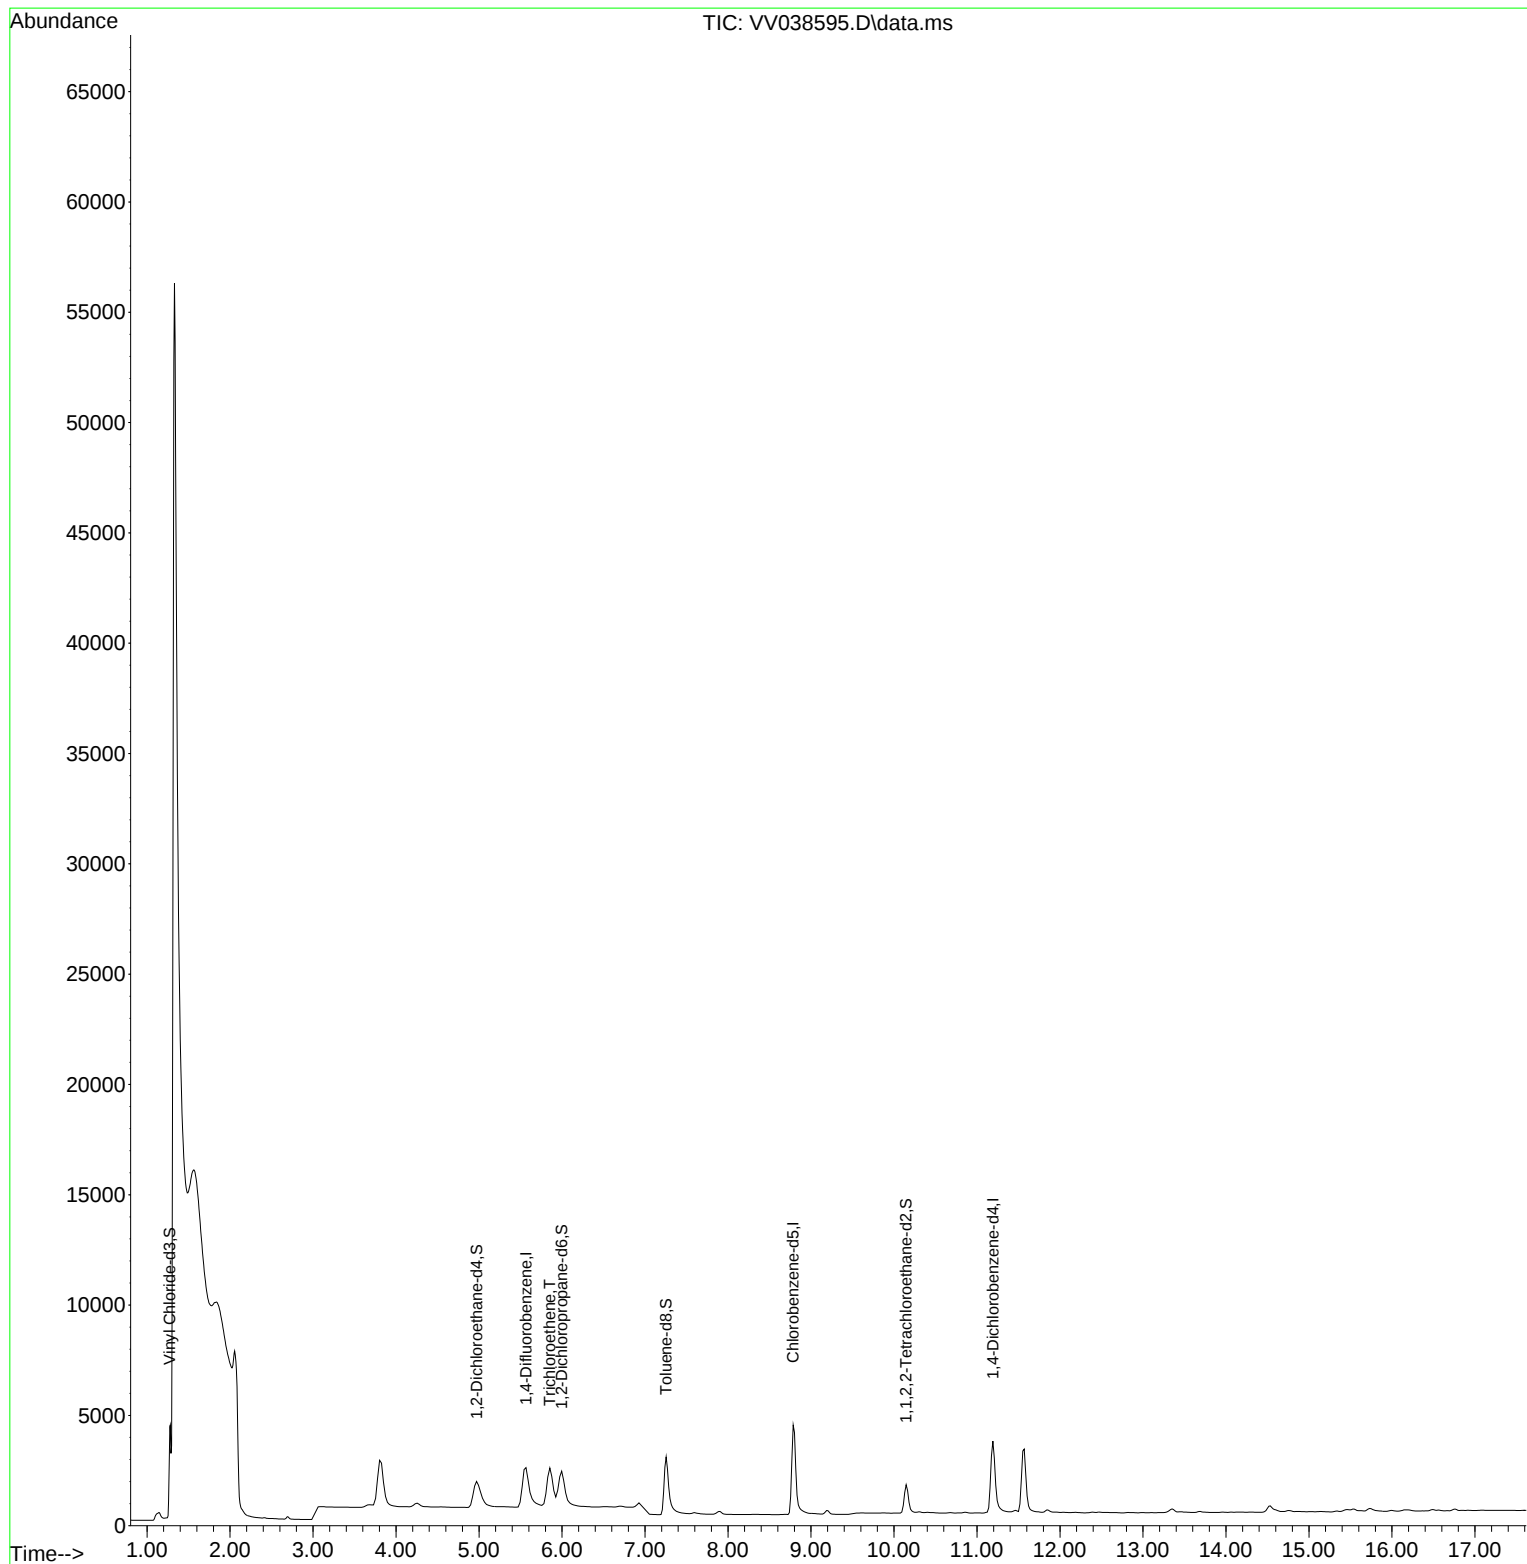

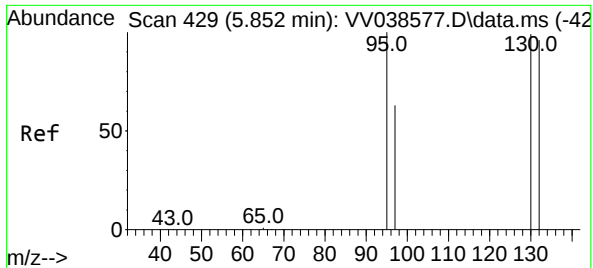

#6
 Trichloroethene
 Concen: 0.400 ug/L
 RT: 5.853 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: VV038595.D
 Acq: 03 Feb 2025 18:55

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZN2

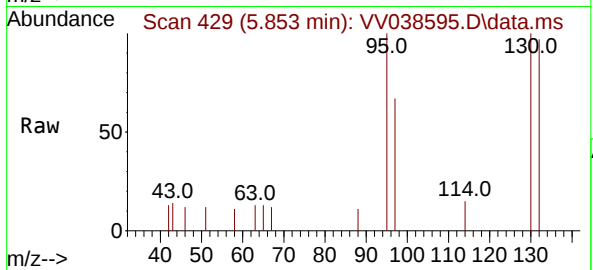

Tgt Ion: 95	Resp: 2617
Ion Ratio	Lower Upper
95 100	
97 67.4	47.9 88.9
132 96.8	68.2 126.6
130 99.6	69.7 129.5

