

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020325\
 Data File : VV038597.D
 Acq On : 03 Feb 2025 19:44
 Operator : SY/MD
 Sample : Q1226-26
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZP4

Quant Time: Feb 04 07:35:16 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 28 08:06:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	6849	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	6902	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	3173	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	2624	0.380	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	76.000%		
4) 1,2-Dichloroethane-d4	4.969	65	2338	0.424	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	84.000%		
7) 1,2-Dichloropropane-d6	5.995	67	2885	0.425	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	86.000%		
8) Toluene-d8	7.254	98	5453	0.401	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	80.000%		
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2539	0.439	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	88.000%		
Target Compounds						
6) Trichloroethene	5.876	95	97	0.017	ug/L	Qvalue # 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020325\
Data File : VV038597.D
Acq On : 03 Feb 2025 19:44
Operator : SY/MD
Sample : Q1226-26
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCZP4


Quant Time: Feb 04 07:35:16 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 28 08:06:10 2025
Response via : Initial Calibration

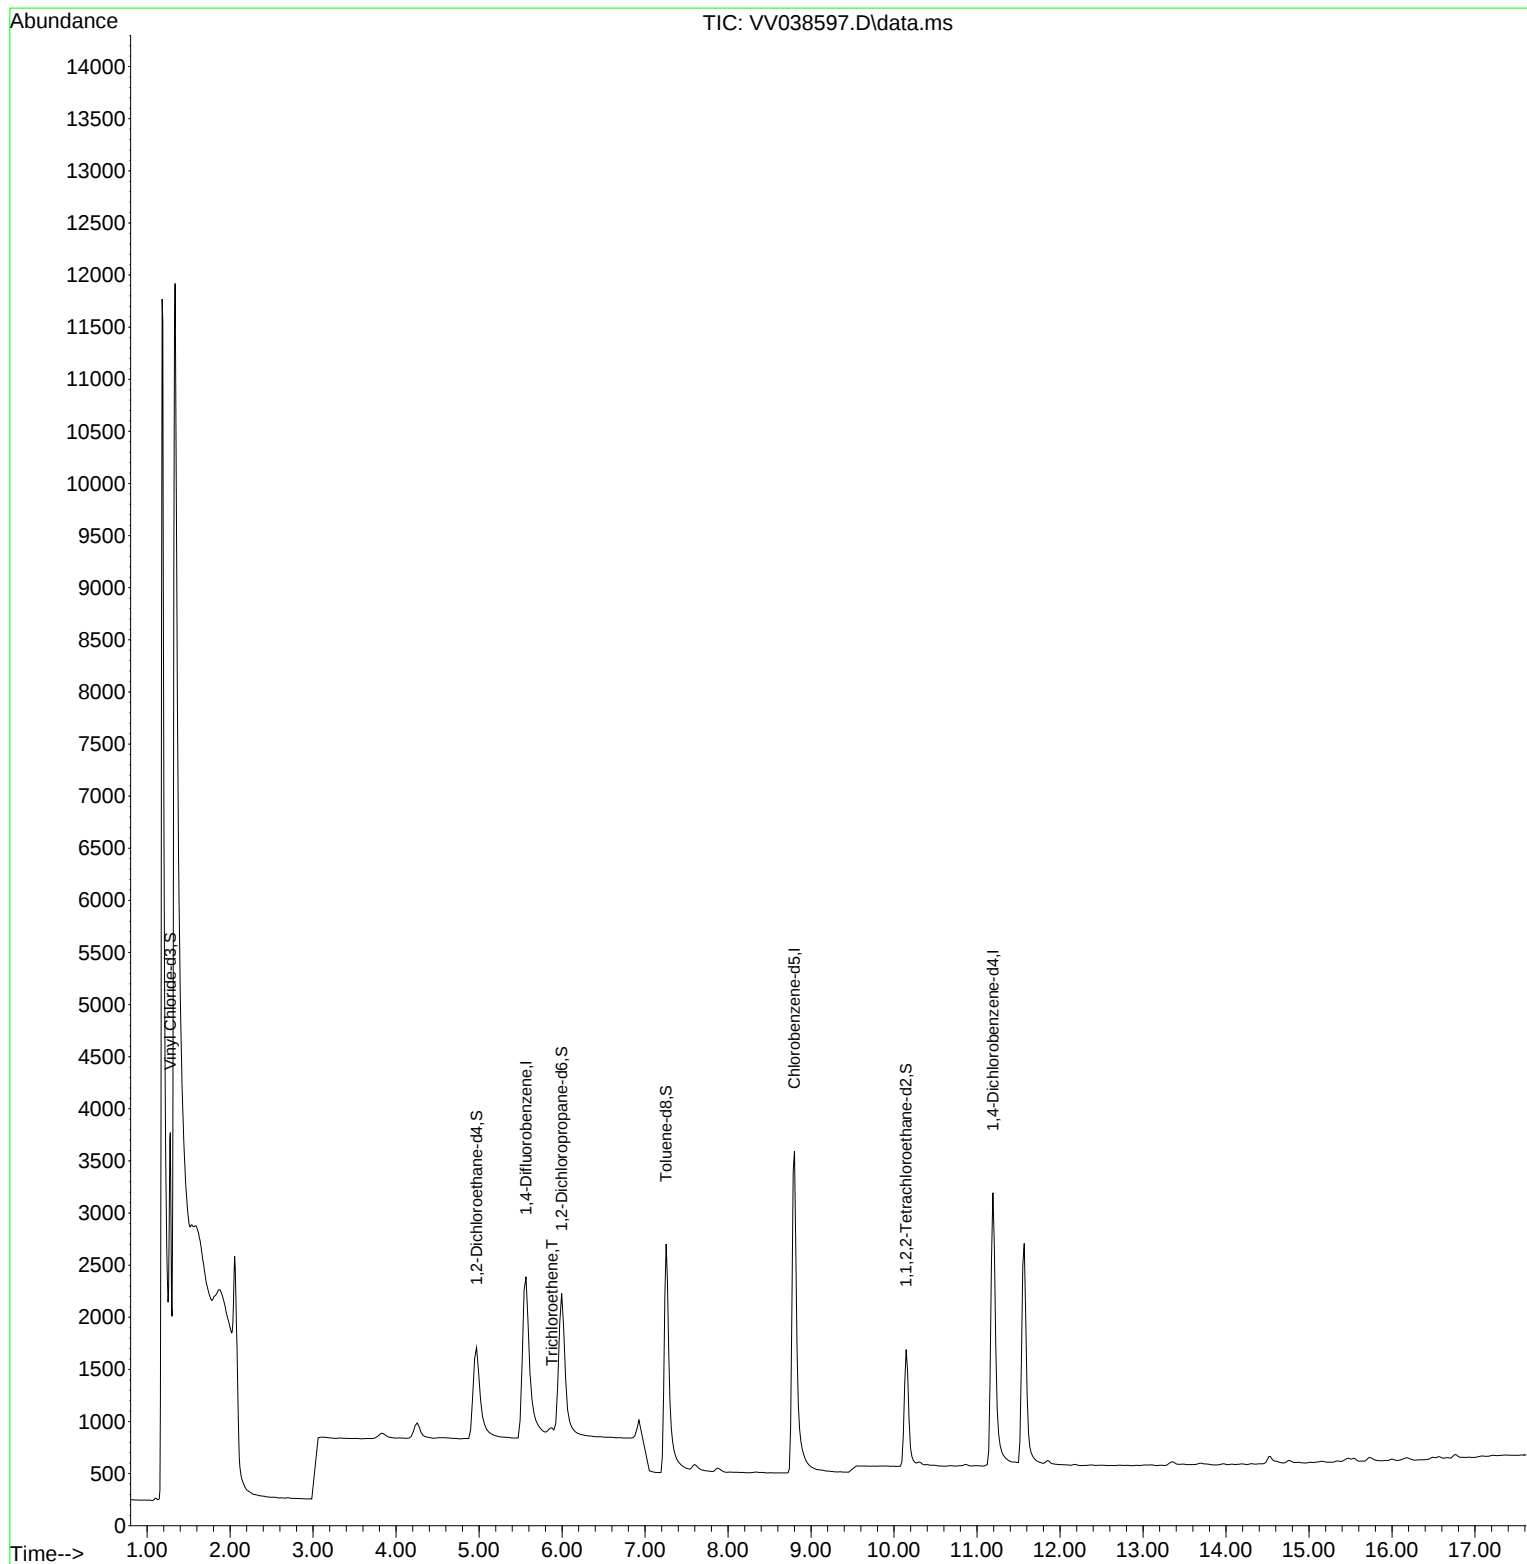

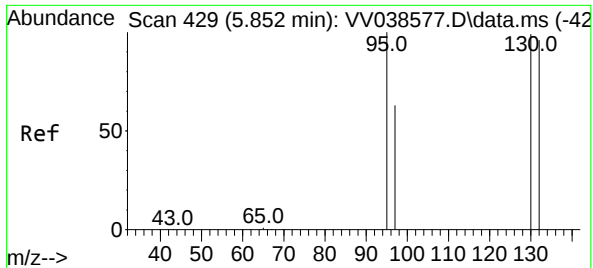

#6
 Trichloroethene
 Concen: 0.017 ug/L
 RT: 5.876 min Scan# 41
 Delta R.T. 0.024 min
 Lab File: VV038597.D
 Acq: 03 Feb 2025 19:44

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZP4

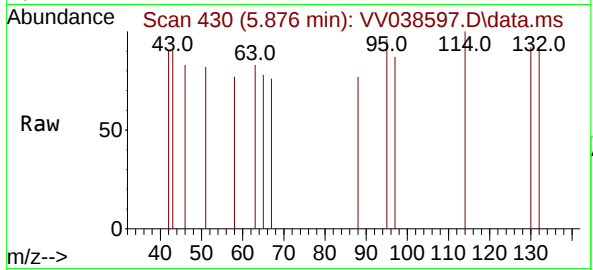

Tgt Ion: 95	Resp: 97
Ion Ratio	Lower Upper
95 100	
97 90.7	47.9 88.9#
132 96.0	68.2 126.6
130 96.0	69.7 129.5

