


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020325\
Data File : VV038576.D
Acq On : 03 Feb 2025 09:57
Operator : SY/MD
Sample : BFB230
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB230

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Title : TRACE VOA SOM01.0
Last Update : Tue Jan 28 08:06:10 2025

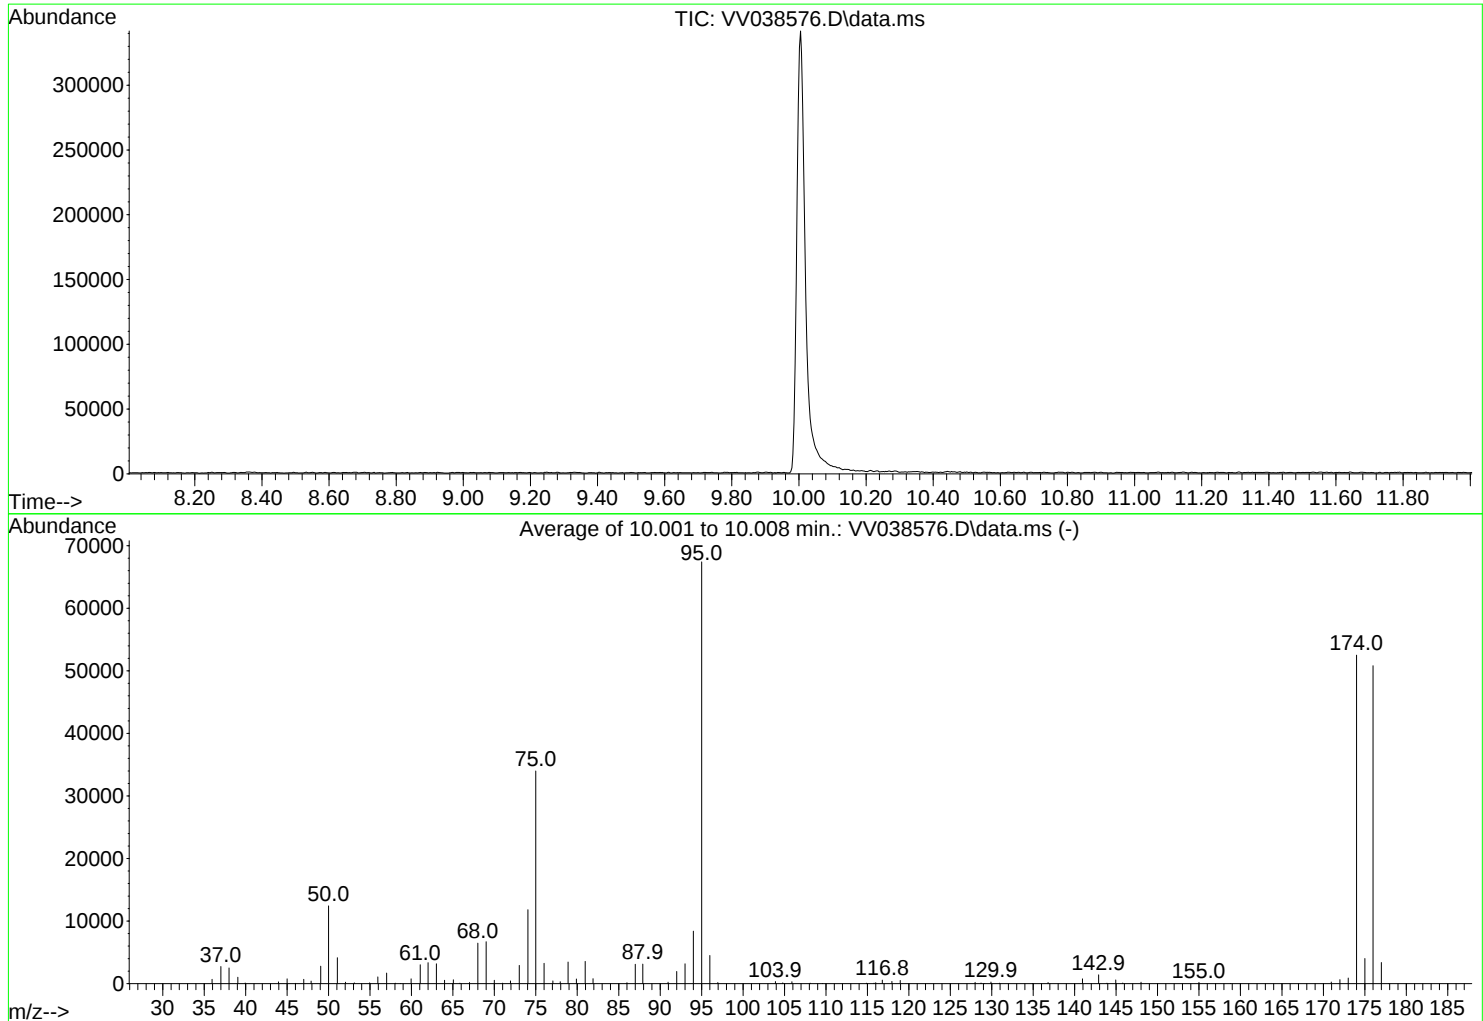

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	12429	PASS
75	95	30	80	50.4	33987	PASS
95	95	100	100	100.0	67424	PASS
96	95	5	9	6.7	4503	PASS
173	174	0.00	2	1.7	907	PASS
174	95	50	120	77.9	52512	PASS
175	174	5	9	7.7	4030	PASS
176	174	95	101	96.8	50821	PASS
177	176	5	9	6.7	3383	PASS

m/z	Abundance
39.90	419.0
43.90	385.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

m/z	Abundance
36.00	728.0
37.00	2929.0
38.00	2546.0
39.10	1067.0
40.00	471.0
44.10	609.0
45.00	749.0
47.00	726.0
47.90	401.0
49.10	2821.0
50.00	12651.0
51.00	4251.0
52.10	236.0
53.10	124.0
54.90	145.0
56.00	1064.0
57.00	1600.0
58.00	139.0
58.70	103.0
60.00	847.0
61.10	3057.0
62.00	3304.0
63.00	3144.0
64.00	576.0
65.10	525.0
67.00	170.0
68.00	6680.0
69.00	6692.0
70.00	583.0
71.00	105.0
72.00	397.0
73.00	2912.0
74.10	11511.0
75.00	33592.0
76.00	3109.0
77.10	431.0
78.00	334.0
78.90	3550.0
79.90	789.0
81.00	3408.0
81.90	711.0
86.00	158.0
87.00	3067.0
87.90	2928.0
91.00	275.0
92.00	1820.0
93.00	3077.0
94.00	8385.0
95.00	67272.0
96.00	4621.0
96.90	157.0
103.90	333.0
104.80	123.0
105.90	332.0
109.60	104.0
114.90	134.0
115.80	209.0
116.80	628.0
117.90	363.0
119.00	612.0
128.00	198.0
129.10	116.0
129.90	256.0
136.80	166.0
140.90	774.0
142.90	1241.0
145.00	637.0
145.80	158.0
148.00	243.0
155.10	208.0
158.80	115.0
171.00	262.0
172.00	587.0
172.90	885.0
174.00	51296.0
175.00	3787.0
176.00	50320.0
177.00	3259.0
177.90	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

m/z	Abundance
36.00	750.0
37.00	2788.0
38.00	2546.0
39.00	1035.0
40.00	516.0
44.10	674.0
45.00	802.0
47.00	666.0
47.90	446.0
49.00	2887.0
50.00	12779.0
51.10	4303.0
52.00	229.0
53.10	111.0
55.00	125.0
55.90	1111.0
57.00	1720.0
58.10	113.0
59.90	796.0
61.10	3036.0
62.00	3467.0
63.00	3242.0
64.00	554.0
65.10	653.0
65.80	110.0
67.00	182.0
68.00	6634.0
69.00	6974.0
70.00	548.0
71.00	106.0
71.90	438.0
73.00	2975.0
74.10	12321.0
75.00	34808.0
76.00	3431.0
77.00	448.0
78.00	340.0
78.90	3543.0
79.90	768.0
80.90	3698.0
81.90	828.0
86.00	166.0
87.00	3144.0
87.90	3307.0
91.00	236.0
92.00	1974.0
93.00	3248.0
94.00	8644.0
95.00	69472.0
96.00	4646.0
97.00	192.0
103.90	351.0
104.80	124.0
105.90	331.0
108.10	106.0
114.90	117.0
116.00	224.0
116.80	588.0
118.00	386.0
119.00	514.0
128.00	216.0
128.70	128.0
129.90	273.0
130.90	114.0
136.80	166.0
140.90	806.0
142.90	1476.0
143.90	122.0
145.00	595.0
145.80	121.0
148.00	240.0
155.00	227.0
157.00	101.0
170.90	262.0
172.00	651.0
173.00	919.0
174.00	53904.0
175.00	4136.0
176.00	52568.0
177.00	3530.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

m/z	Abundance
35.90	620.0
37.00	2491.0
38.00	2448.0
39.00	1010.0
40.00	548.0
44.00	707.0
45.00	726.0
46.00	127.0
47.00	669.0
47.90	419.0
49.00	2638.0
50.00	11857.0
51.10	3894.0
52.00	223.0
53.10	122.0
55.00	116.0
55.90	1053.0
57.00	1756.0
59.90	701.0
61.00	2954.0
62.00	3311.0
63.00	3157.0
64.00	469.0
65.00	673.0
65.90	111.0
67.00	181.0
68.00	6126.0
69.00	6424.0
70.00	477.0
71.90	479.0
73.00	2828.0
74.00	11658.0
75.00	33560.0
76.00	3207.0
77.00	446.0
77.90	282.0
78.90	3254.0
79.90	697.0
80.90	3583.0
81.90	847.0
86.00	146.0
87.00	3112.0
87.90	3134.0
90.90	218.0
92.00	2006.0
93.00	3173.0
94.00	8122.0
95.00	65528.0
96.00	4243.0
97.00	180.0
103.90	328.0
104.80	123.0
105.90	291.0
108.10	121.0
116.00	257.0
116.80	481.0
118.00	346.0
118.90	393.0
128.00	242.0
128.70	157.0
129.90	254.0
131.00	141.0
134.90	112.0
136.80	203.0
141.00	724.0
142.90	1527.0
143.90	137.0
144.90	526.0
148.00	220.0
154.90	181.0
170.90	224.0
172.00	669.0
173.10	916.0
174.00	52336.0
175.00	4166.0
176.00	49576.0
177.00	3359.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230