

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020425\
 Data File : VV038604.D
 Acq On : 04 Feb 2025 16:04
 Operator : SY/MD
 Sample : Q1226-08RE
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZP0RE

Quant Time: Feb 05 07:30:47 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 28 08:06:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	5392	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	5416	0.500	ug/L	-0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	2624	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	1941	0.357	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	72.000%		
4) 1,2-Dichloroethane-d4	4.970	65	1593	0.367	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	74.000%		
7) 1,2-Dichloropropane-d6	5.996	67	1898	0.357	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	72.000%		
8) Toluene-d8	7.254	98	3425	0.321	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	64.000%#		
10) 1,1,2,2-Tetrachloroeth...	10.146	84	1810	0.399	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	80.000%		
Target Compounds						
6) Trichloroethene	5.829	95	8023	1.793	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020425\
Data File : VV038604.D
Acq On : 04 Feb 2025 16:04
Operator : SY/MD
Sample : Q1226-08RE
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCZP0RE

Quant Time: Feb 05 07:30:47 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 28 08:06:10 2025
Response via : Initial Calibration

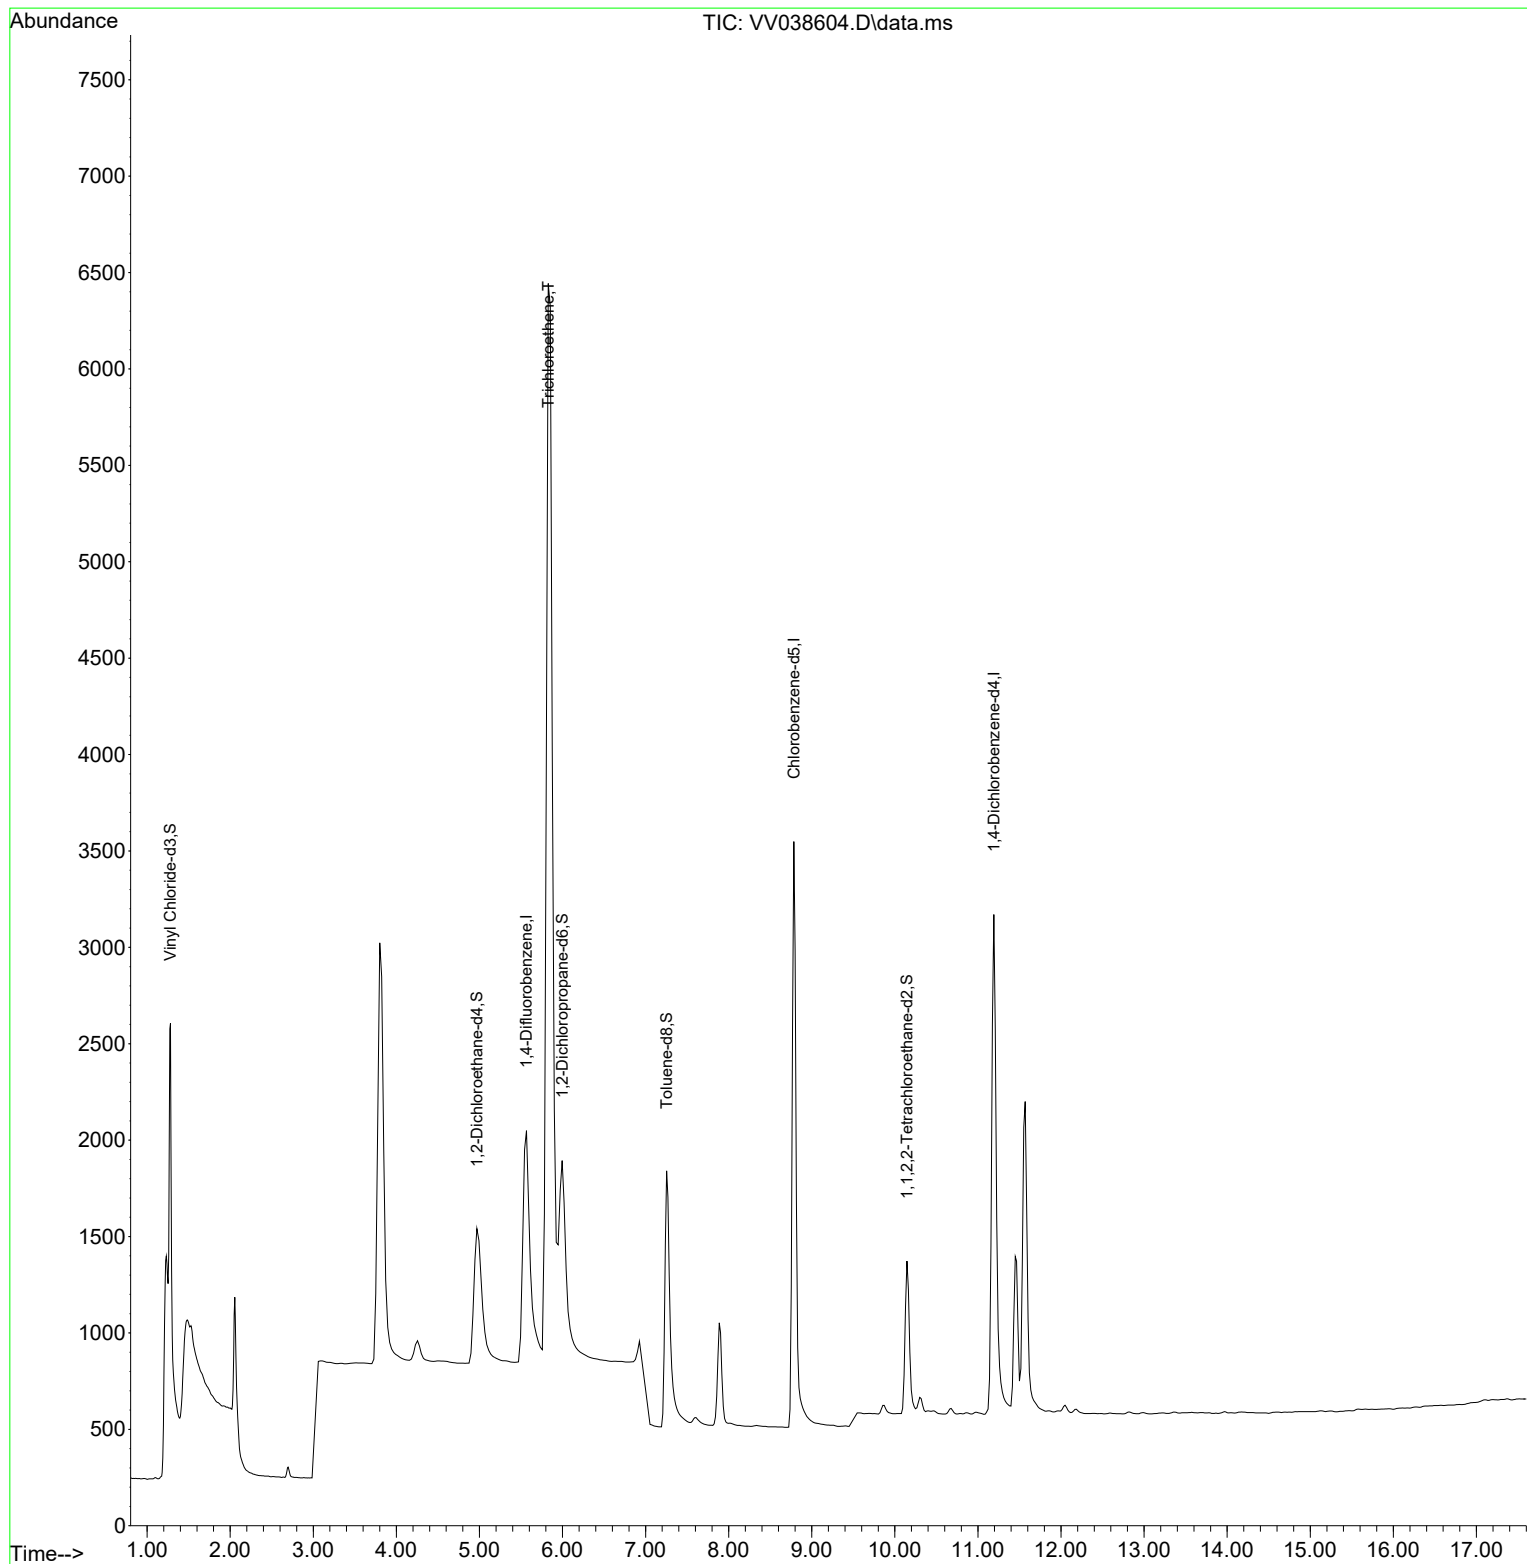

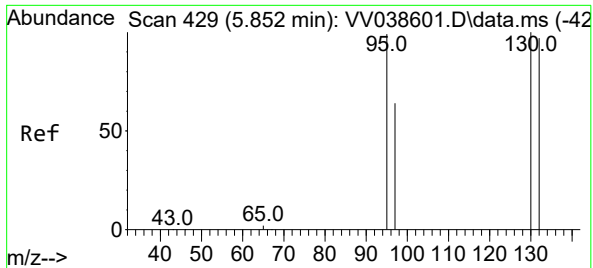

Trichloroethene

Concen: 1.793 ug/L

RT: 5.829 min Scan# 41

Delta R.T. -0.023 min

Lab File: VV038604.D


Acq: 04 Feb 2025 16:04

Instrument :

MSVOA_V

ClientSampleId :

DCZP0RE

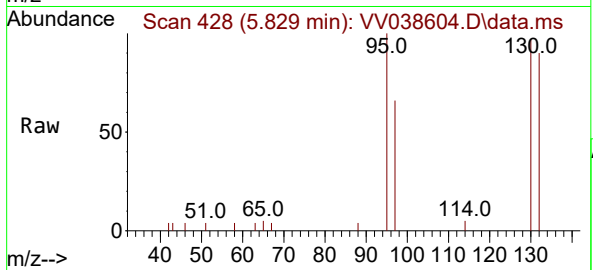

Tgt Ion: 95 Resp: 8023

Ion Ratio Lower Upper

95 100

97 65.7 47.9 88.9

132 89.6 68.2 126.6

130 96.9 69.7 129.5

