

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020425\
 Data File : VV038605.D
 Acq On : 04 Feb 2025 16:28
 Operator : SY/MD
 Sample : Q1226-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZP5

Quant Time: Feb 05 07:30:59 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 28 08:06:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	5499	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	5522	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	2647	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	2000	0.361	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	72.000%
4) 1,2-Dichloroethane-d4	4.969	65	1781	0.402	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	80.000%
7) 1,2-Dichloropropane-d6	5.995	67	2123	0.391	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	78.000%
8) Toluene-d8	7.253	98	3926	0.361	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	72.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2072	0.448	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	90.000%
Target Compounds						
6) Trichloroethene	5.852	95	4235	0.928	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020425\
Data File : VV038605.D
Acq On : 04 Feb 2025 16:28
Operator : SY/MD
Sample : Q1226-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCZP5

Quant Time: Feb 05 07:30:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 28 08:06:10 2025
Response via : Initial Calibration

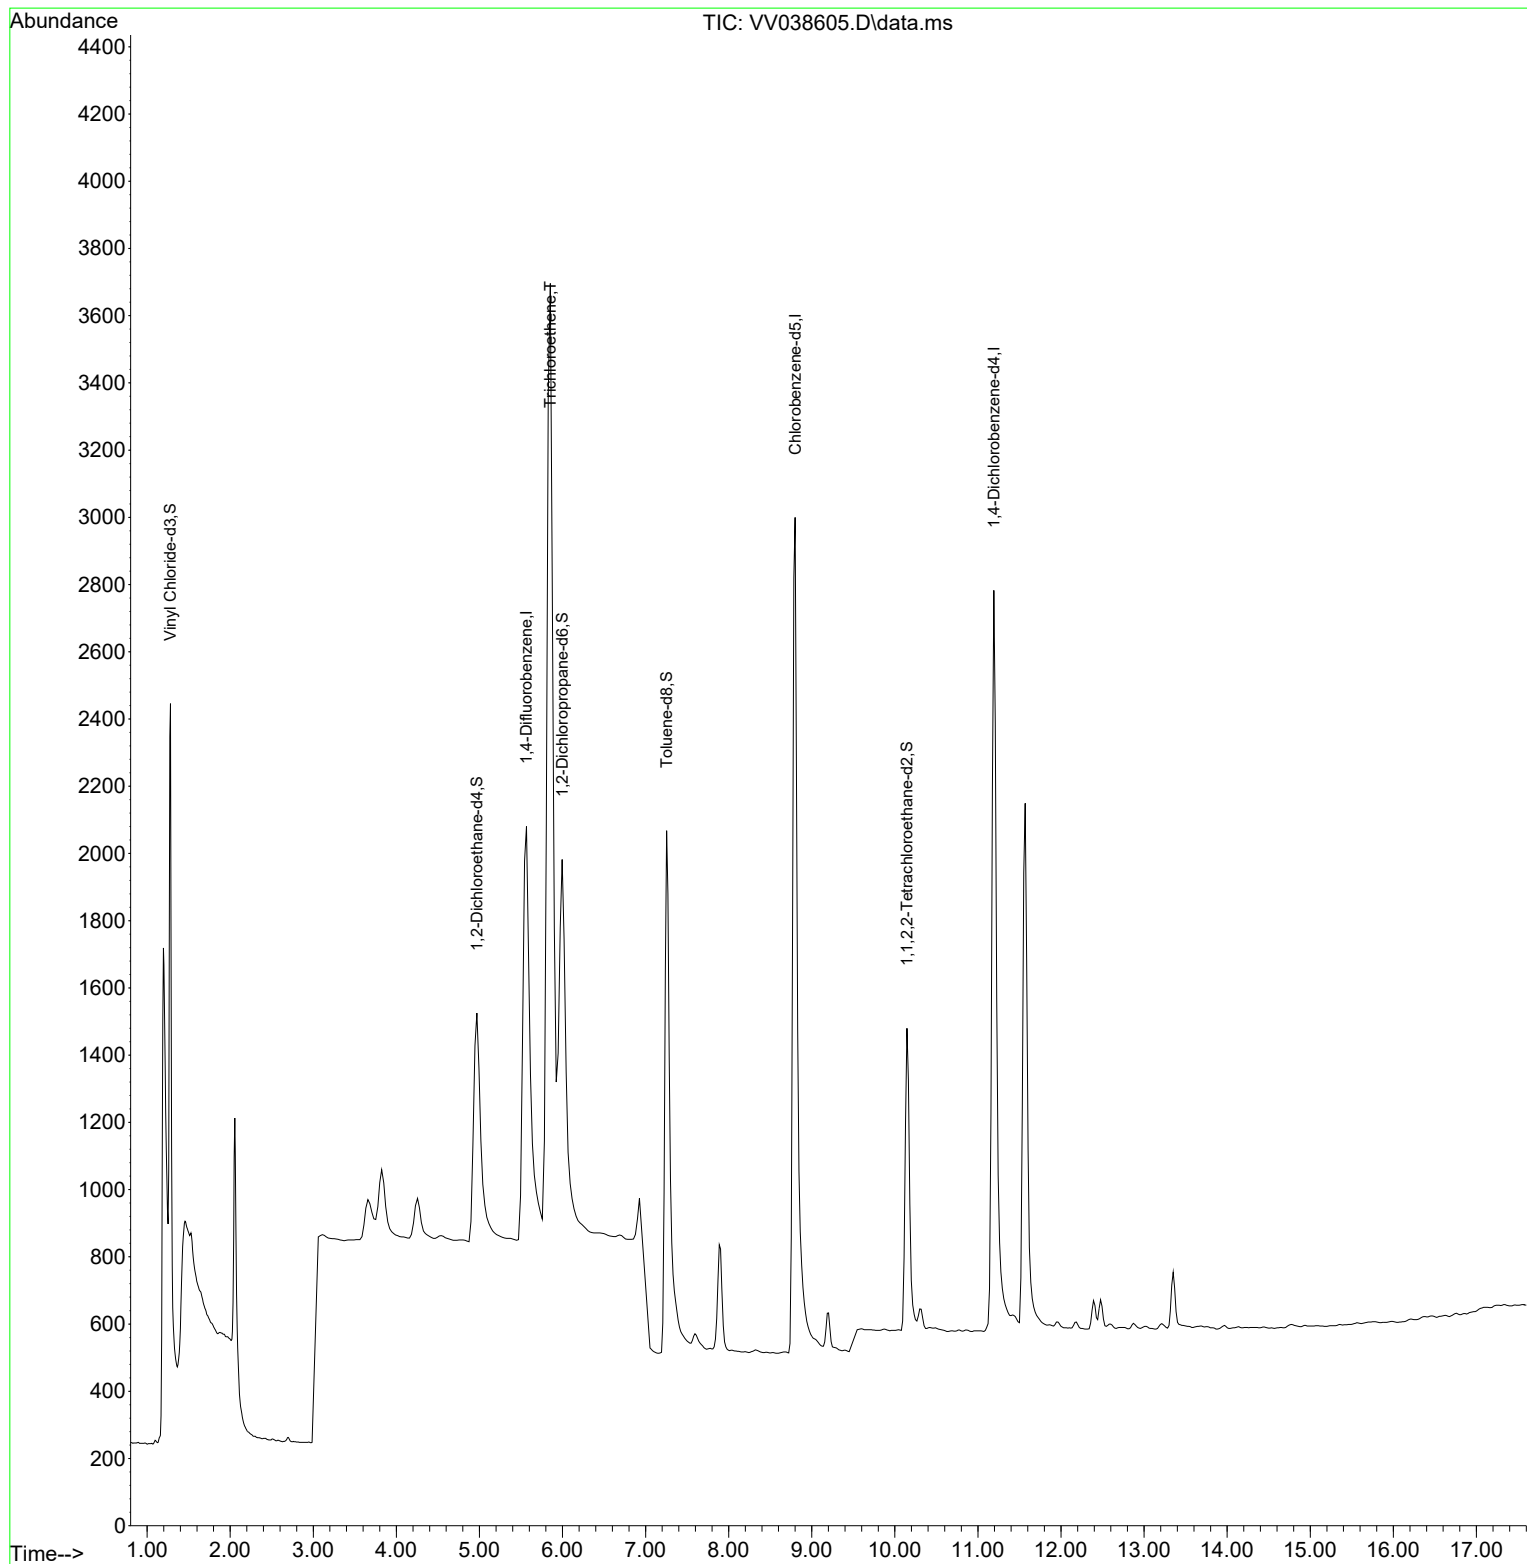

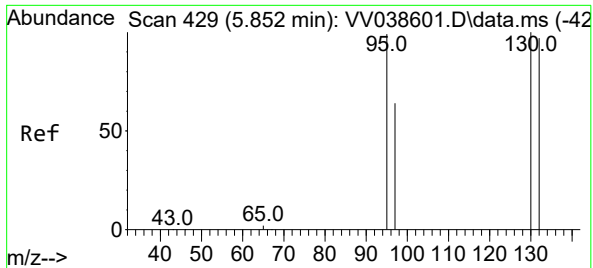

Trichloroethene

Concen: 0.928 ug/L

RT: 5.852 min Scan# 41

Delta R.T. -0.000 min

Lab File: VV038605.D


Acq: 04 Feb 2025 16:28

Instrument :

MSVOA_V

ClientSampleId :

DCZP5

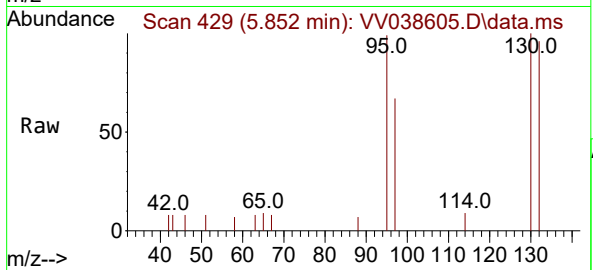

Tgt Ion: 95 Resp: 4235

Ion Ratio Lower Upper

95 100

97 66.9 47.9 88.9

132 96.5 68.2 126.6

130 100.6 69.7 129.5

