

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020425\
 Data File : VV038608.D
 Acq On : 04 Feb 2025 17:41
 Operator : SY/MD
 Sample : Q1226-11DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZK4DL

Quant Time: Feb 05 07:31:35 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 28 08:06:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	5161	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	5342	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	2504	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	2101	0.404	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	80.000%		
4) 1,2-Dichloroethane-d4	4.970	65	1873	0.451	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	90.000%		
7) 1,2-Dichloropropane-d6	5.996	67	2202	0.419	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	84.000%		
8) Toluene-d8	7.254	98	4055	0.385	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	78.000%		
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2180	0.487	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	98.000%		
Target Compounds					Qvalue	
6) Trichloroethene	5.829	95	5427	1.230	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020425\
Data File : VV038608.D
Acq On : 04 Feb 2025 17:41
Operator : SY/MD
Sample : Q1226-11DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCZK4DL


Quant Time: Feb 05 07:31:35 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 28 08:06:10 2025
Response via : Initial Calibration

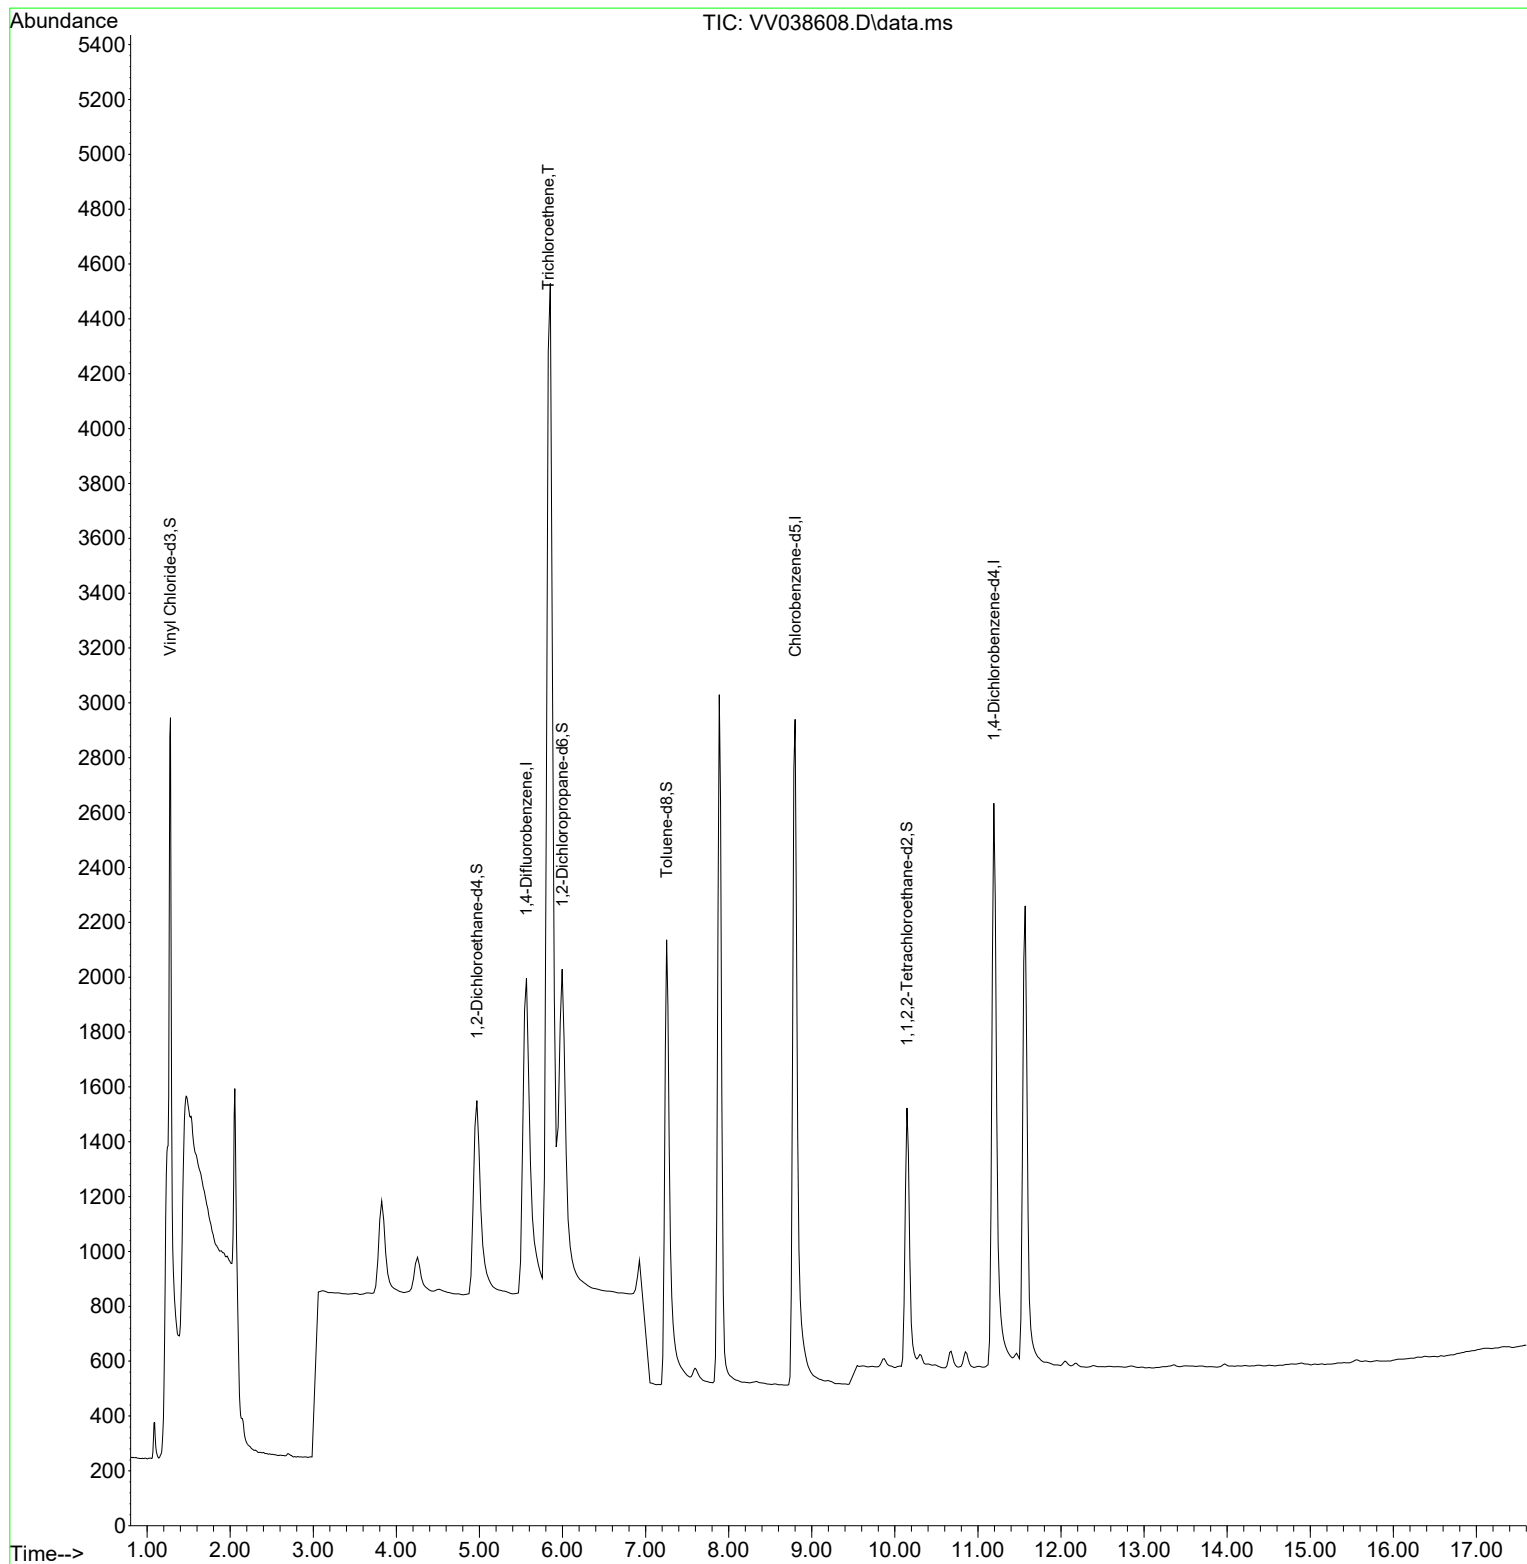

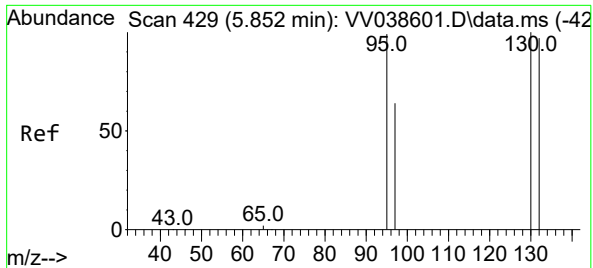

#6
 Trichloroethene
 Concen: 1.230 ug/L
 RT: 5.829 min Scan# 41
 Delta R.T. -0.024 min
 Lab File: VV038608.D
 Acq: 04 Feb 2025 17:41

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZK4DL

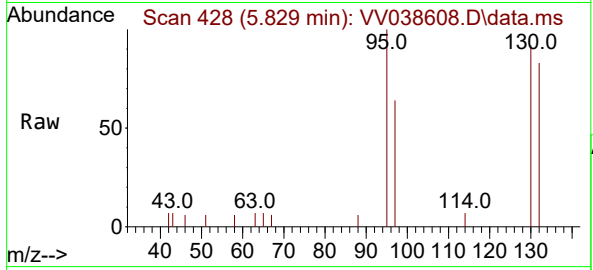

Tgt Ion: 95 Resp: 5427

Ion	Ratio	Lower	Upper
95	100		
97	64.3	47.9	88.9
132	82.9	68.2	126.6
130	91.6	69.7	129.5

