

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020425\
 Data File : VV038612.D
 Acq On : 04 Feb 2025 19:19
 Operator : SY/MD
 Sample : Q1226-23
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZN9

Quant Time: Feb 05 07:32:25 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 28 08:06:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	8000	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	8571	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	4137	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	3265	0.405	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	80.000%		
4) 1,2-Dichloroethane-d4	4.969	65	2597	0.403	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	80.000%		
7) 1,2-Dichloropropane-d6	5.995	67	3116	0.370	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	74.000%		
8) Toluene-d8	7.253	98	6289	0.372	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	74.000%		
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2779	0.387	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	78.000%		
Target Compounds						
6) Trichloroethene	5.828	95	86633	12.236	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020425\
Data File : VV038612.D
Acq On : 04 Feb 2025 19:19
Operator : SY/MD
Sample : Q1226-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCZN9

Quant Time: Feb 05 07:32:25 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 28 08:06:10 2025
Response via : Initial Calibration

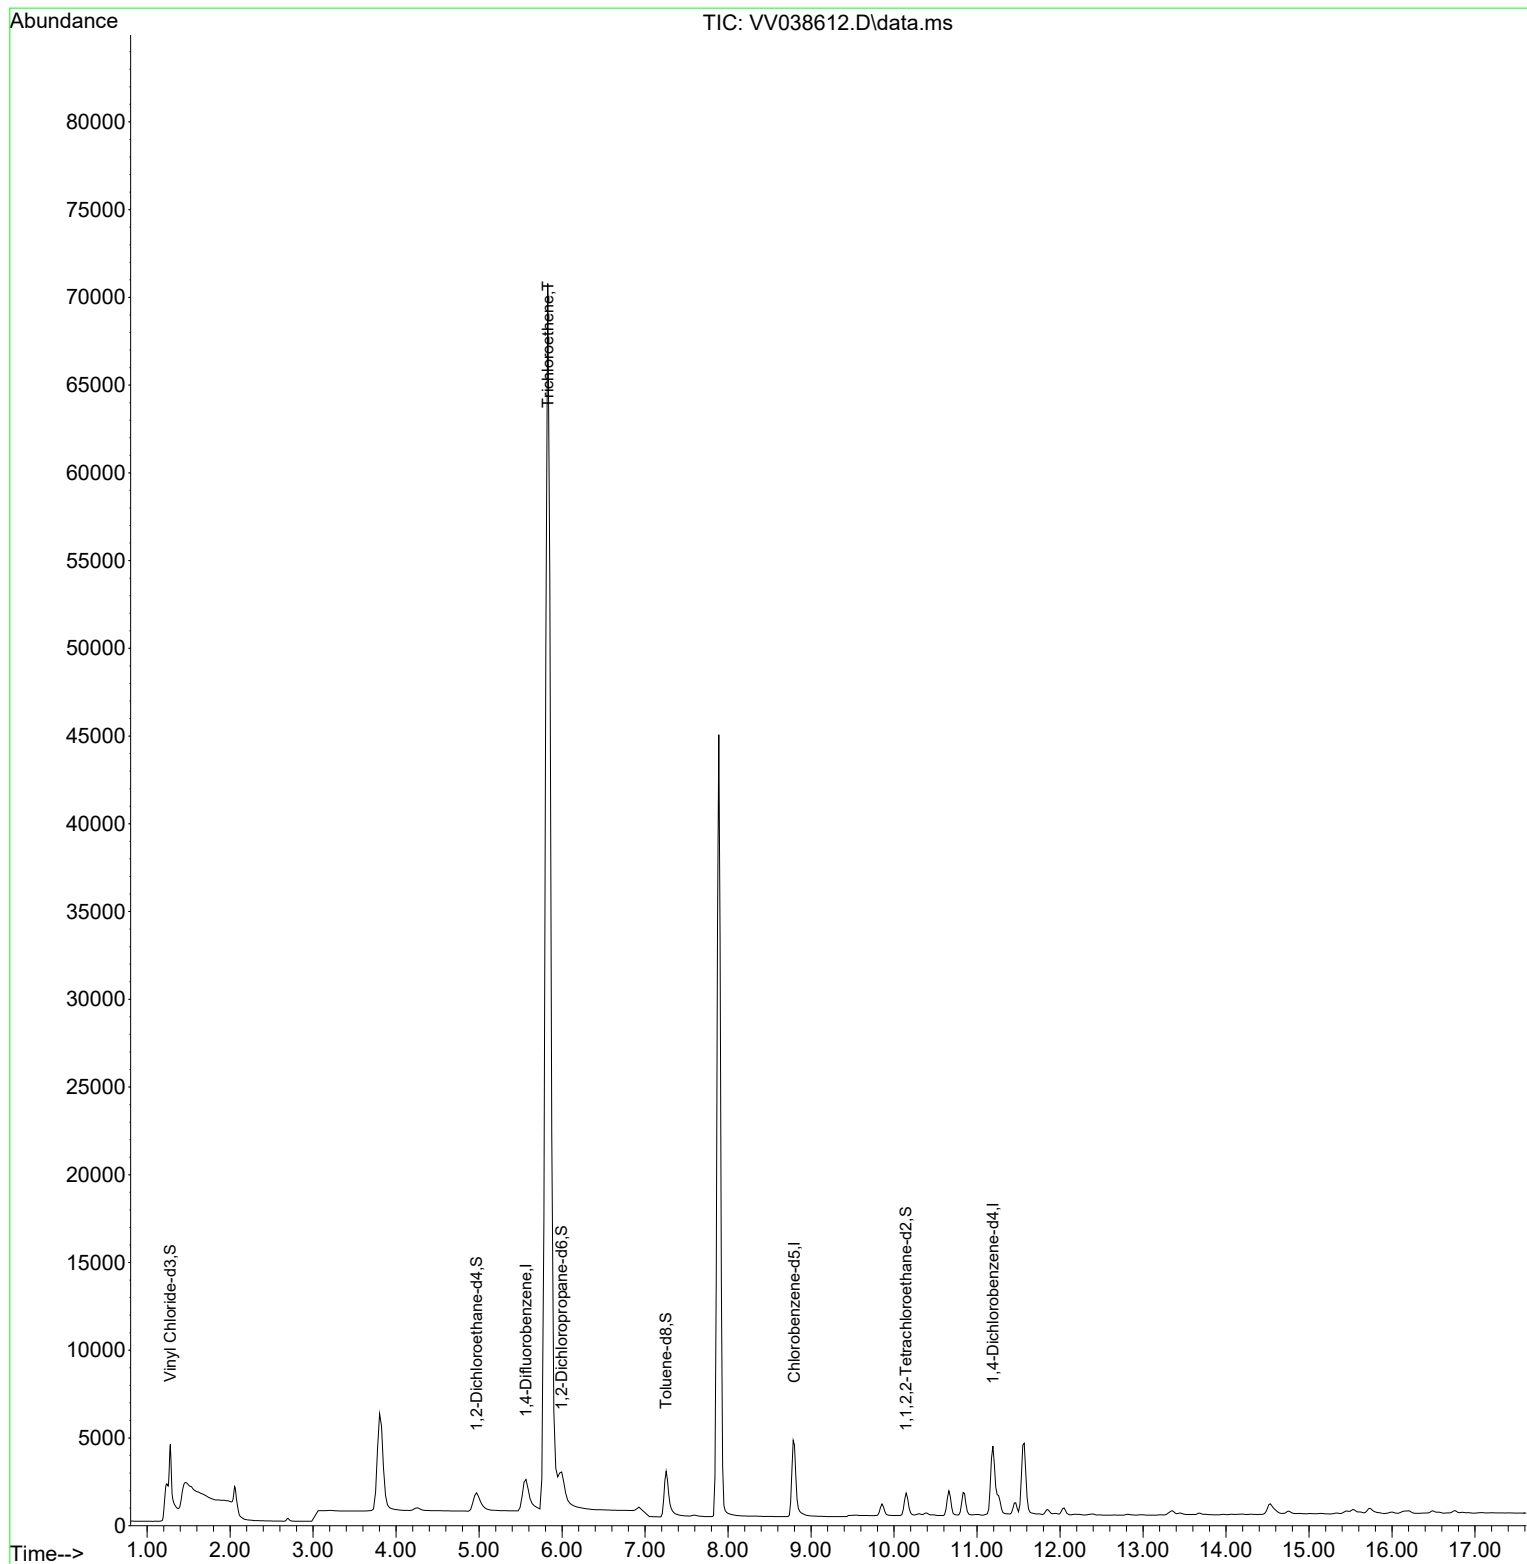

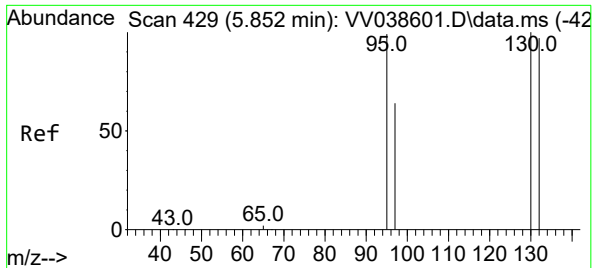

Trichloroethene

Concen: 12.236 ug/L

RT: 5.828 min Scan# 41

Delta R.T. -0.024 min

Lab File: VV038612.D


Acq: 04 Feb 2025 19:19

Instrument :

MSVOA_V

ClientSampleId :

DCZN9

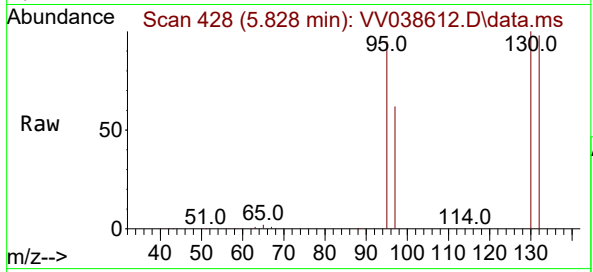

Tgt Ion: 95 Resp: 86633

Ion Ratio Lower Upper

95 100

97 65.5 47.9 88.9

132 103.0 68.2 126.6

130 105.3 69.7 129.5

