

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020425\
 Data File : VV038614.D
 Acq On : 04 Feb 2025 20:07
 Operator : SY/MD
 Sample : Q1226-25
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZN7

Quant Time: Feb 05 08:02:08 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 28 08:06:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	6865	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	6898	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	3159	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	3107	0.449	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	90.000%		
4) 1,2-Dichloroethane-d4	4.969	65	2295	0.415	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	84.000%		
7) 1,2-Dichloropropane-d6	5.995	67	2856	0.421	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	84.000%		
8) Toluene-d8	7.253	98	5467	0.402	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	80.000%		
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2568	0.444	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	88.000%		
Target Compounds						
6) Trichloroethene	5.876	95	115	0.020	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020425\
Data File : VV038614.D
Acq On : 04 Feb 2025 20:07
Operator : SY/MD
Sample : Q1226-25
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCZN7


Quant Time: Feb 05 08:02:08 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 28 08:06:10 2025
Response via : Initial Calibration

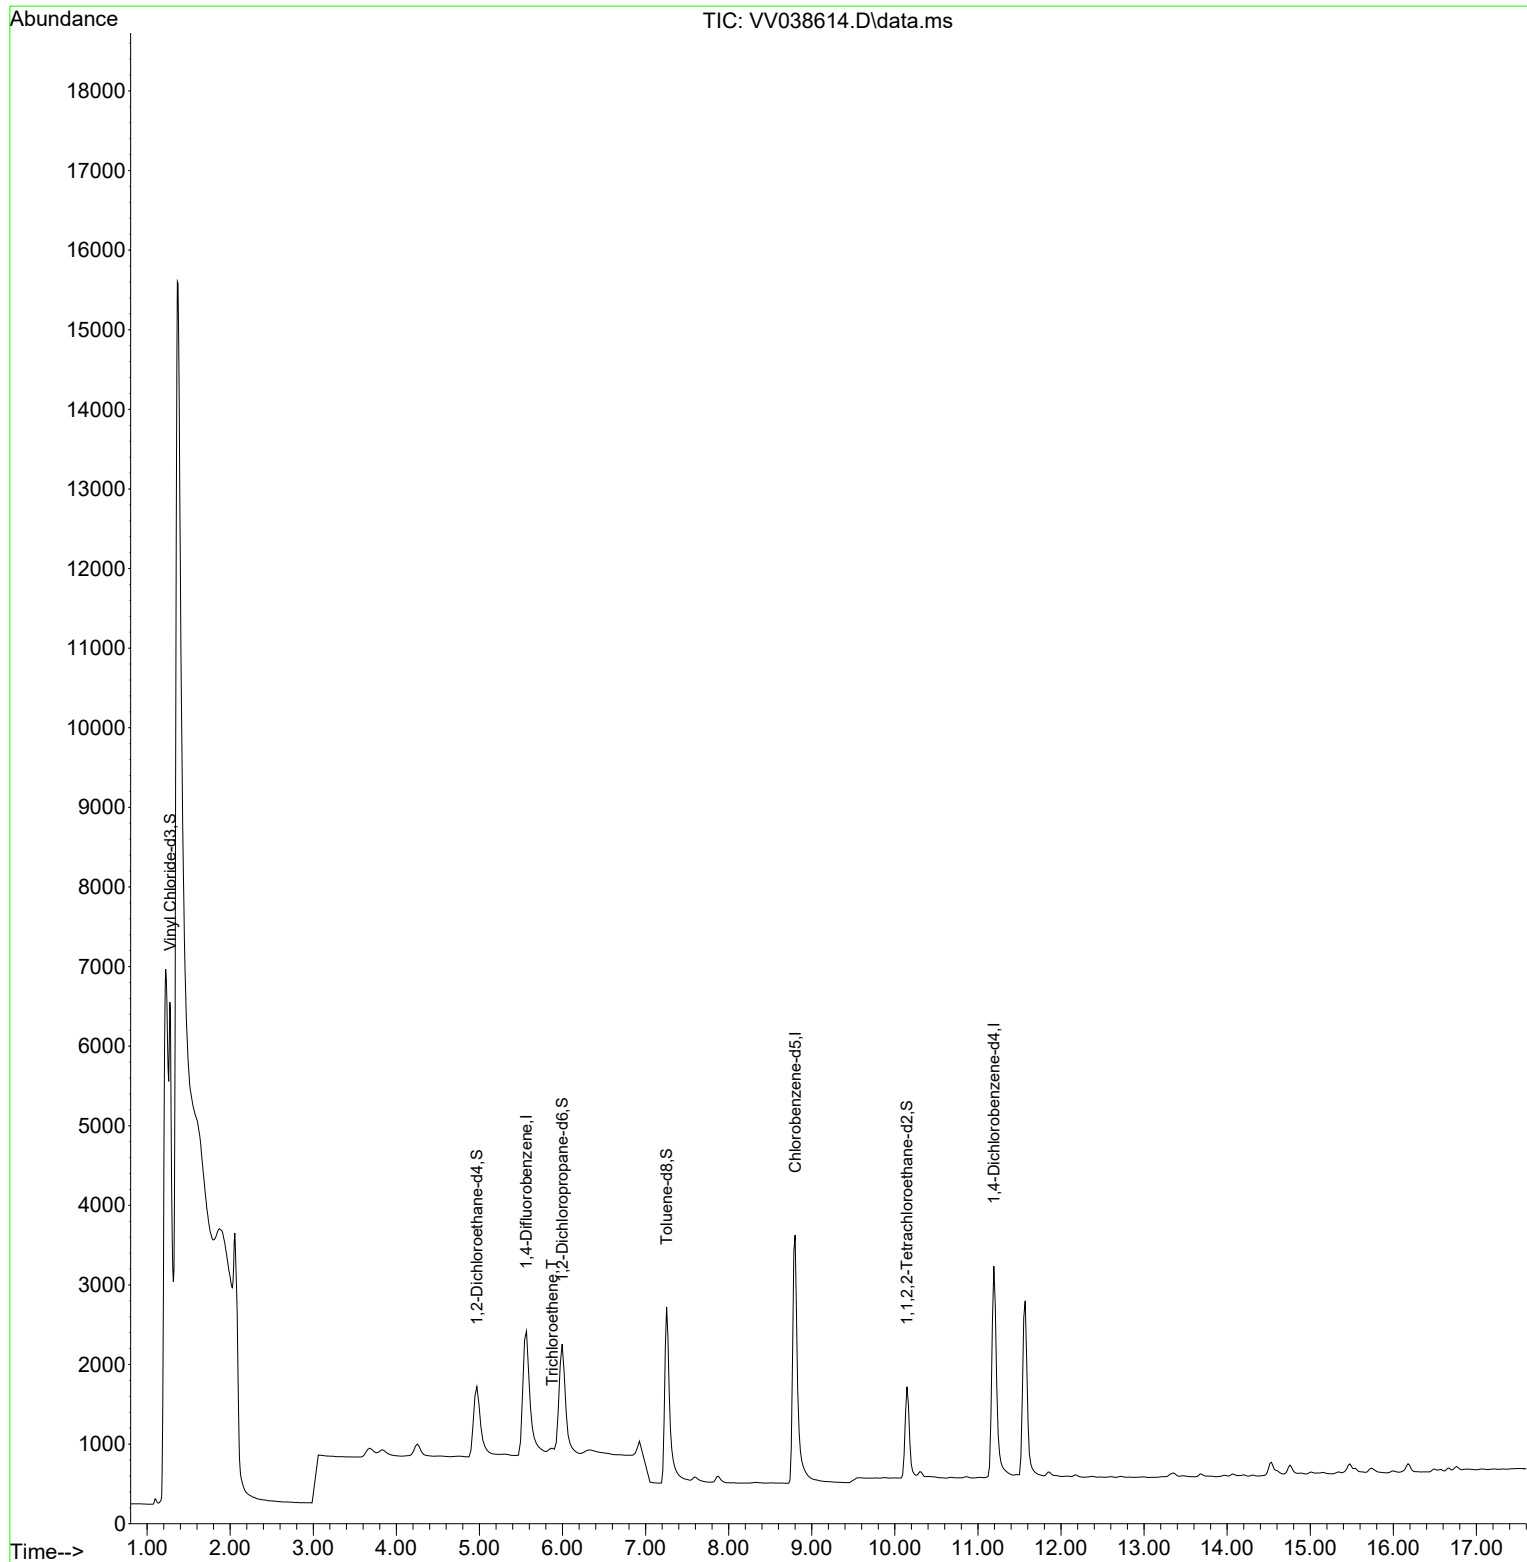

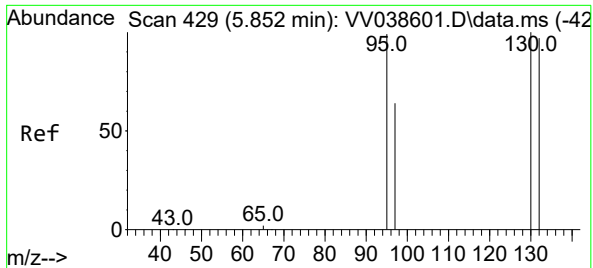

Trichloroethene
 Concen: 0.020 ug/L
 RT: 5.876 min Scan# 41
 Delta R.T. 0.024 min
 Lab File: VV038614.D
 Acq: 04 Feb 2025 20:07

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZN7

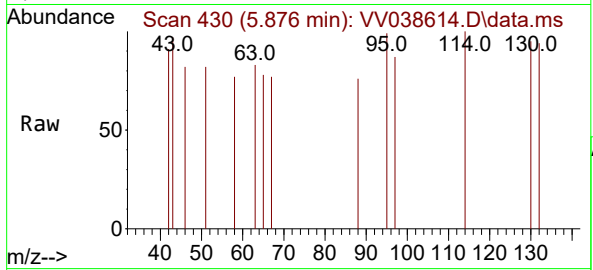

Tgt Ion: 95	Resp: 115
Ion Ratio	Lower Upper
95	100
97	88.3 47.9 88.9
132	94.8 68.2 126.6
130	96.1 69.7 129.5

