
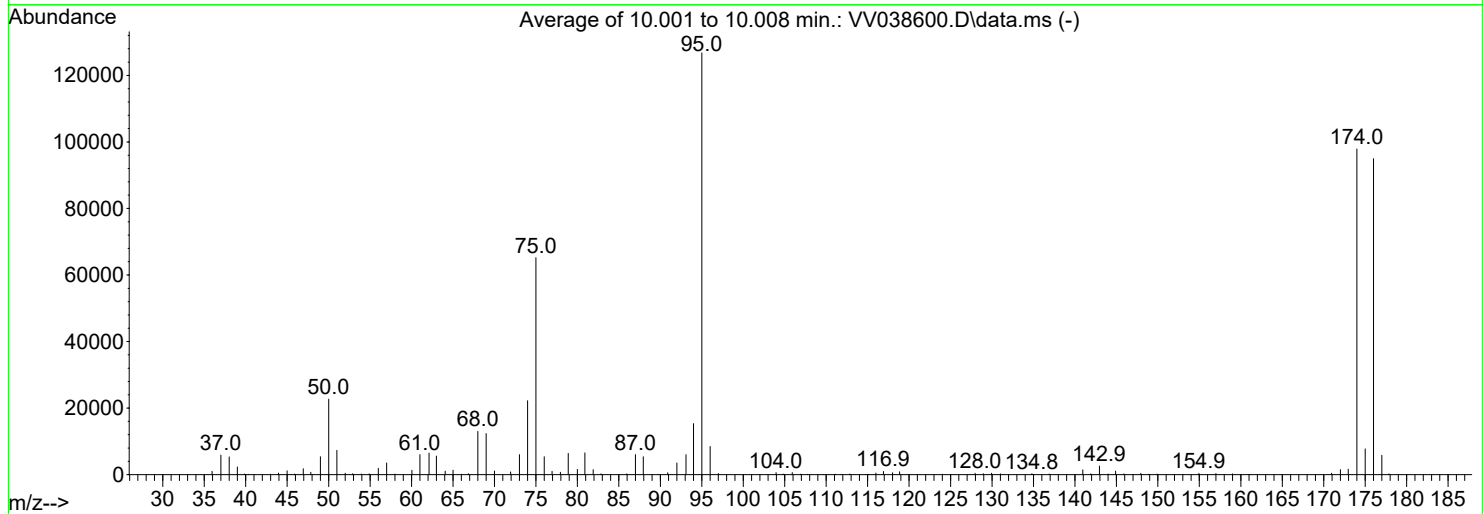


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020425\
Data File : VV038600.D
Acq On : 04 Feb 2025 13:00
Operator : SY/MD
Sample : BFB231
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB231

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Title : TRACE VOA SOM01.0
Last Update : Tue Jan 28 08:06:10 2025

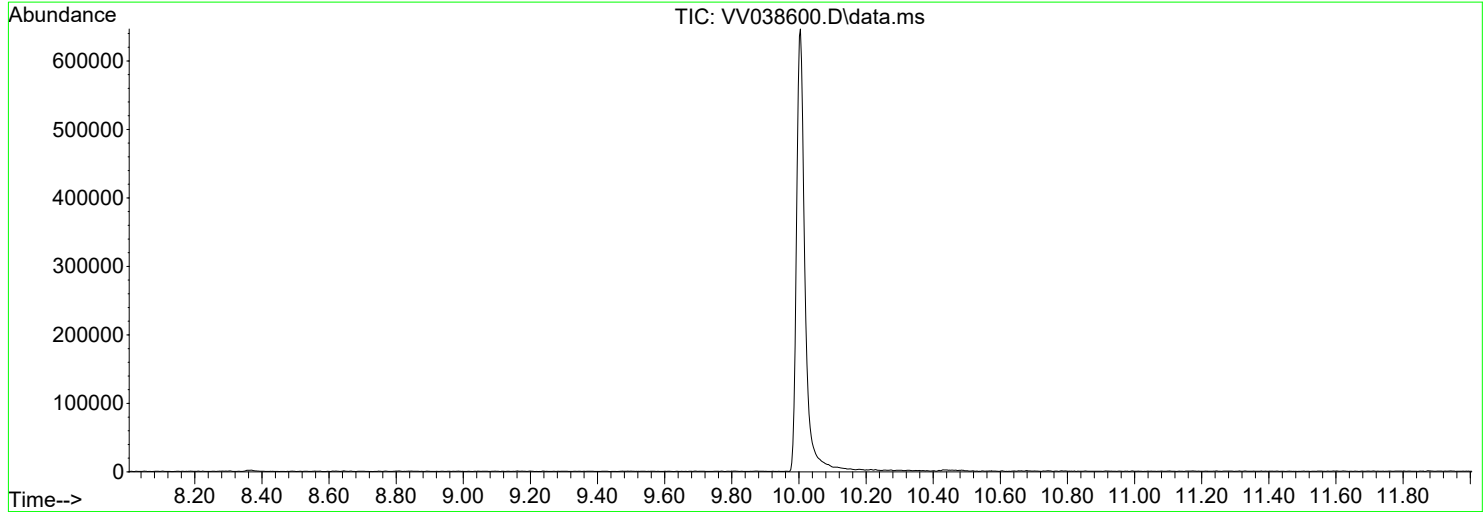

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	22707	PASS
75	95	30	80	51.5	65227	PASS
95	95	100	100	100.0	126773	PASS
96	95	5	9	6.7	8468	PASS
173	174	0.00	2	1.7	1619	PASS
174	95	50	120	77.2	97877	PASS
175	174	5	9	7.9	7746	PASS
176	174	95	101	97.0	94971	PASS
177	176	5	9	6.1	5832	PASS

m/z	Abundance
36.00	144.0
39.80	235.0
43.90	487.0
77.20	140.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231

m/z	Abundance
35.90	1145.0
37.00	6135.0
38.00	5640.0
39.00	2454.0
39.90	476.0
40.30	337.0
43.00	176.0
44.00	998.0
45.00	1049.0
45.90	220.0
46.90	1800.0
47.90	775.0
49.00	5714.0
50.00	23632.0
51.00	7839.0
52.00	361.0
52.90	260.0
53.90	214.0
54.90	321.0
56.00	2139.0
57.00	3574.0
58.00	212.0
60.00	1323.0
61.00	6416.0
62.10	6504.0
63.00	5665.0
64.00	1177.0
65.00	1381.0
66.10	168.0
66.80	307.0
68.00	13481.0
69.00	12801.0
70.00	1068.0
72.00	807.0
73.00	6325.0
74.00	23416.0
75.00	67432.0
76.00	5477.0
76.90	974.0
78.00	695.0
78.90	6757.0
80.00	1630.0
80.90	6609.0
81.90	1456.0
82.90	221.0
85.90	228.0
87.00	6214.0
88.00	5815.0
90.90	659.0
92.00	3570.0
93.10	5821.0
94.00	15179.0
95.00	129104.0
96.00	8393.0
97.00	348.0
103.90	636.0
104.80	257.0
105.90	597.0
106.90	190.0
111.20	153.0
112.80	194.0
115.10	119.0
116.00	550.0
116.90	965.0
118.00	586.0
118.80	891.0
124.00	119.0
127.90	425.0
129.00	230.0
129.90	409.0
131.10	262.0
134.80	341.0
136.90	187.0
141.00	1618.0
141.90	225.0
143.00	2432.0
144.00	217.0
144.90	1172.0
145.90	237.0
148.00	370.0
148.90	151.0
149.90	196.0
155.00	405.0
157.00	432.0
159.00	249.0
160.90	119.0
170.90	405.0
172.00	1358.0
172.90	1572.0
174.00	96344.0
175.00	7548.0
176.00	94984.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231

177.005818.0

177.90237.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231

m/z	Abundance
35.90	1202.0
37.00	6093.0
38.00	5619.0
39.00	2347.0
39.90	461.0
43.00	171.0
44.00	1014.0
45.00	1201.0
45.90	205.0
47.00	1816.0
47.90	770.0
49.00	5594.0
50.00	23272.0
51.00	7546.0
52.00	426.0
52.90	319.0
54.00	192.0
54.90	250.0
56.00	1978.0
57.00	3591.0
58.00	218.0
60.00	1360.0
61.00	6234.0
62.10	6785.0
63.00	5640.0
64.10	1073.0
65.00	1368.0
66.00	156.0
66.90	299.0
68.00	13323.0
69.00	12602.0
70.00	1188.0
71.90	824.0
73.00	6210.0
74.00	22904.0
75.00	67112.0
76.00	5557.0
76.90	1049.0
78.00	761.0
78.90	6632.0
80.00	1640.0
80.90	6774.0
81.90	1528.0
82.80	234.0
86.00	258.0
87.00	6261.0
88.00	5405.0
89.80	124.0
90.90	625.0
92.00	3567.0
93.10	6320.0
94.00	15722.0
95.00	130800.0
96.00	8759.0
97.00	382.0
104.00	670.0
104.80	299.0
105.90	617.0
106.90	162.0
107.70	109.0
111.10	182.0
111.80	117.0
112.80	232.0
115.10	122.0
116.00	515.0
116.90	1005.0
118.00	616.0
118.90	878.0
124.00	155.0
128.00	444.0
128.90	288.0
129.90	418.0
131.00	257.0
134.80	287.0
136.90	226.0
140.90	1489.0
141.90	274.0
142.90	2711.0
144.00	201.0
144.90	1115.0
145.90	247.0
147.00	111.0
148.00	427.0
148.90	170.0
149.90	223.0
153.10	125.0
155.00	417.0
157.00	366.0
159.00	258.0
161.10	122.0
171.00	430.0
172.00	1525.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231

173.00	1658.0
174.00	100688.0
175.00	8018.0
176.00	98368.0
177.00	6055.0
177.80	246.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231

m/z	Abundance
36.00	1115.0
37.00	5374.0
38.00	4838.0
39.00	2090.0
39.90	374.0
43.00	105.0
44.00	953.0
45.00	1169.0
45.90	216.0
47.00	1763.0
47.80	659.0
49.00	4854.0
50.00	21216.0
51.00	6553.0
52.00	470.0
52.90	254.0
54.00	191.0
54.90	207.0
56.00	1727.0
57.00	3352.0
58.00	201.0
60.10	1229.0
61.00	5380.0
62.10	6190.0
63.00	5415.0
64.10	886.0
65.00	1264.0
66.00	150.0
66.90	269.0
68.00	12223.0
69.00	11744.0
70.00	1136.0
71.90	807.0
73.00	5574.0
74.00	20384.0
75.00	61136.0
76.00	5176.0
77.00	983.0
77.90	664.0
78.90	5854.0
80.00	1575.0
80.90	6264.0
81.90	1487.0
82.90	221.0
86.00	201.0
87.00	5516.0
87.90	5017.0
90.90	496.0
92.00	3349.0
93.10	5949.0
94.00	15197.0
95.00	120416.0
96.00	8253.0
97.00	328.0
104.00	636.0
105.00	286.0
105.90	647.0
106.90	162.0
107.80	151.0
109.70	103.0
111.00	191.0
111.80	140.0
112.90	229.0
114.80	120.0
116.00	468.0
116.90	1001.0
118.00	570.0
118.90	835.0
124.00	137.0
128.00	476.0
128.90	342.0
130.00	432.0
130.90	245.0
134.80	245.0
136.90	257.0
140.90	1297.0
141.90	236.0
142.90	2682.0
144.00	169.0
144.90	926.0
145.90	221.0
147.10	115.0
147.90	393.0
148.90	151.0
149.90	189.0
153.10	131.0
154.90	387.0
157.00	264.0
159.00	198.0
161.10	146.0
171.00	490.0
172.00	1539.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231

173.00	1626.0
174.00	96600.0
175.00	7673.0
176.00	91560.0
177.00	5624.0
177.90	216.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231