

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW020524\
 Data File : VW033979.D
 Acq On : 05 Feb 2024 11:34
 Operator : SY/MD
 Sample : P1289-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG6

Quant Time: Feb 06 05:12:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Feb 06 05:11:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	101347	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	93816	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	45953	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	27618	3.519	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	70.400%
7) Chloroethane-d5	1.535	69	24199	3.520	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	70.400%
11) 1,1-Dichloroethene-d2	2.059	65	13538	3.576	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.600%
20) 2-Butanone-d5	3.805	46	37448	28.408	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	56.820%
24) Chloroform-d	4.249	84	50113	3.514	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	70.200%
26) 1,2-Dichloroethane-d4	4.944	65	23668	3.551	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.000%
32) Benzene-d6	4.960	84	100799	3.581	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	71.600%
36) 1,2-Dichloropropane-d6	5.989	67	28064	3.567	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	71.400%
41) Toluene-d8	7.243	98	93556	3.617	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.400%
43) trans-1,3-Dichloroprop...	7.561	79	9382	3.158	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	63.200%
46) 2-Hexanone-d5	8.027	63	28666	27.029	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	54.060%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	15086	3.163	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	63.200%#
66) 1,2-Dichlorobenzene-d4	11.561	152	30950	3.703	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	74.000%#
Target Compounds					Qvalue	
13) Acetone	2.127	43	4965	4.965	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020524\
Data File : VV033979.D
Acq On : 05 Feb 2024 11:34
Operator : SY/MD
Sample : P1289-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG6

Quant Time: Feb 06 05:12:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Feb 06 05:11:25 2024
Response via : Initial Calibration

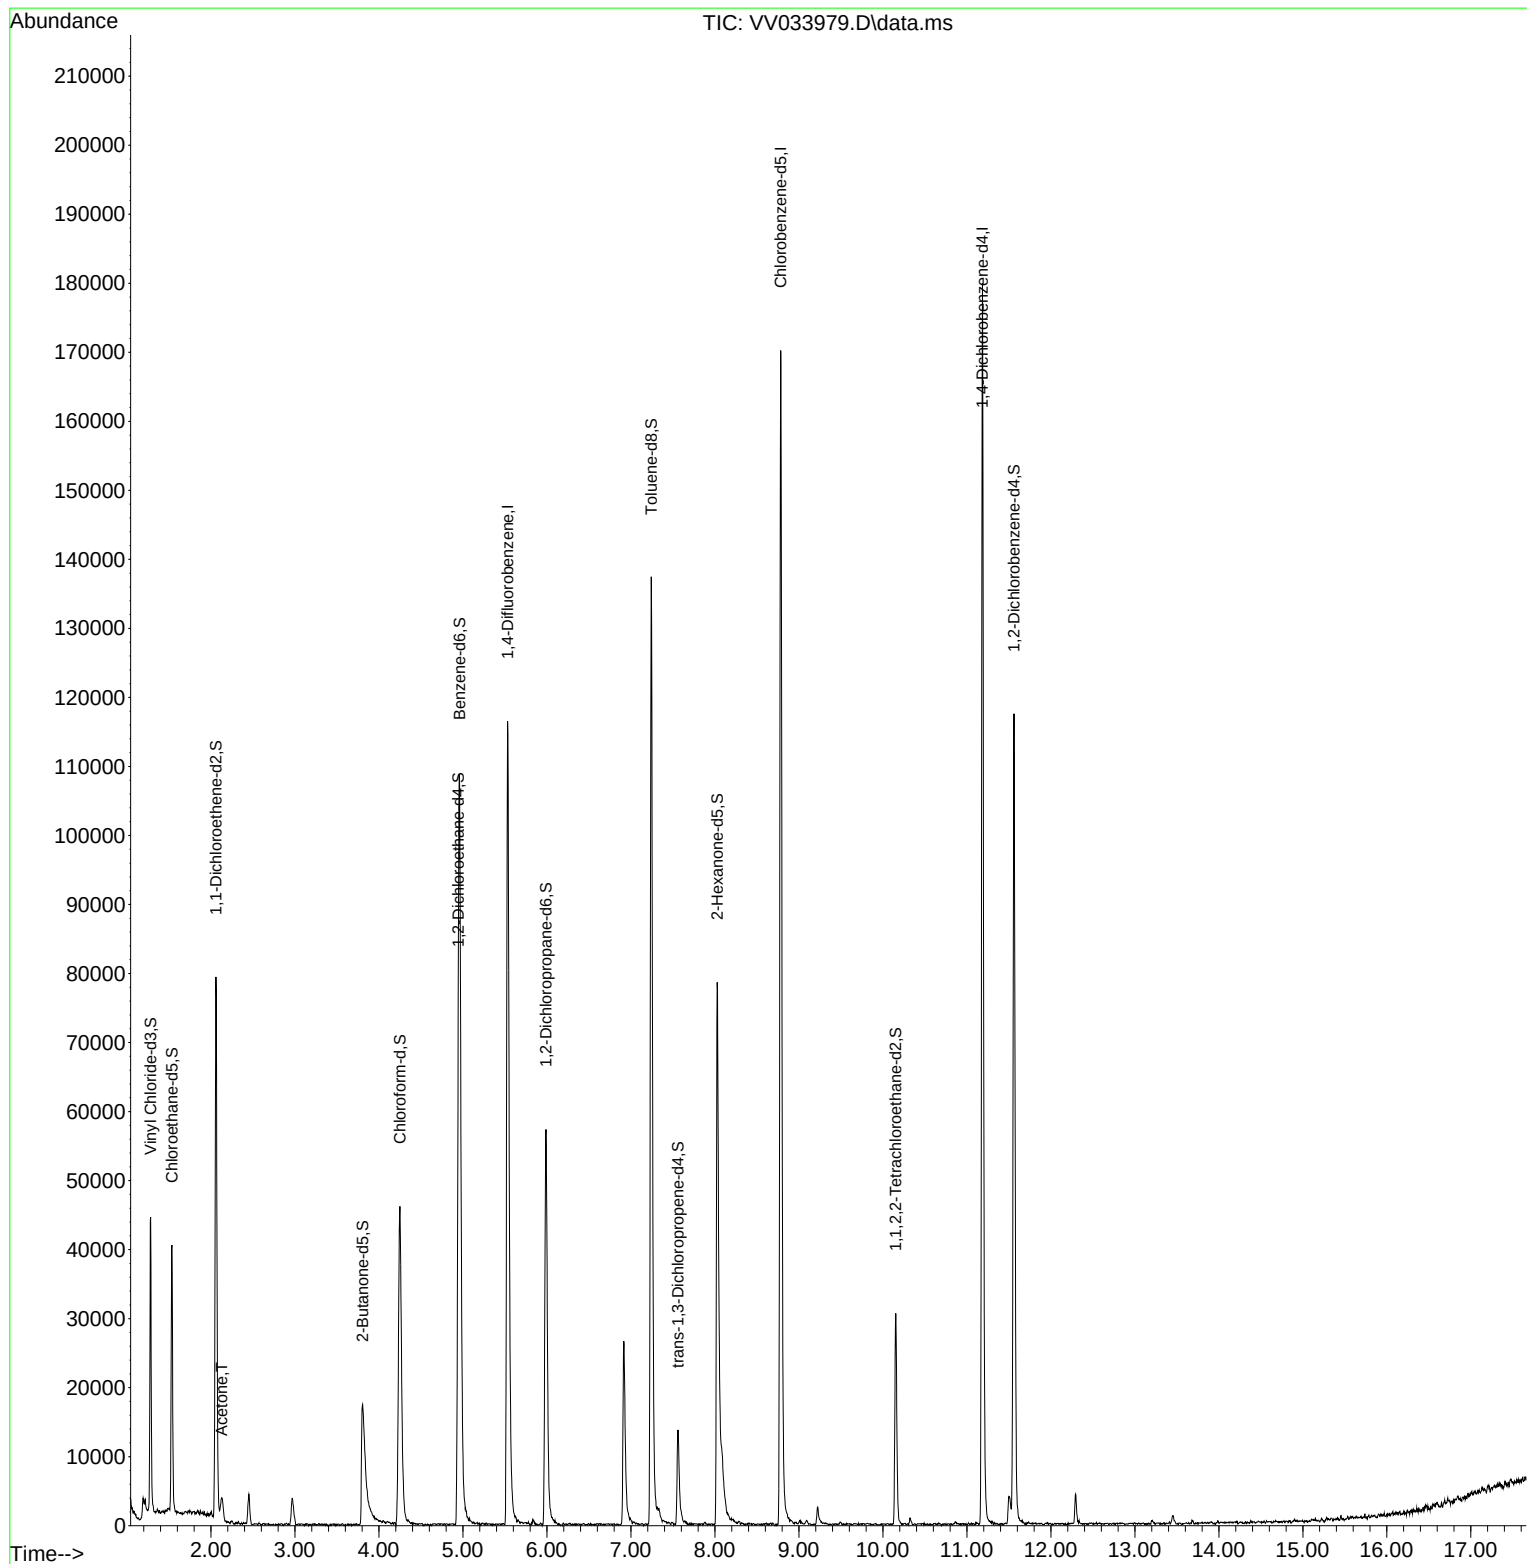

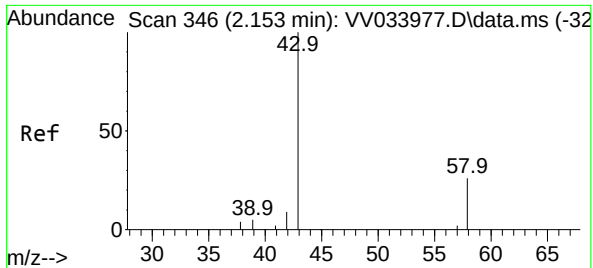

#13
Acetone
Concen: 4.965 ug/L
RT: 2.127 min Scan# 31
Delta R.T. -0.026 min
Lab File: VV033979.D
Acq: 05 Feb 2024 11:34

Instrument :
MSVOA_V
ClientSampleId :
C0AG6

Tgt Ion: 43 Resp: 4965
Ion Ratio Lower Upper
43 100
58 11.8 0.0 13.8

