

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW020524\
 Data File : VW033980.D
 Acq On : 05 Feb 2024 11:58
 Operator : SY/MD
 Sample : P1289-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG7

Quant Time: Feb 06 05:12:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Feb 06 05:11:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	98633	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	91665	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	46606	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	30435	3.984	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.600%
7) Chloroethane-d5	1.536	69	27442	4.101	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.000%
11) 1,1-Dichloroethene-d2	2.063	65	15243	4.138	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.800%
20) 2-Butanone-d5	3.806	46	47695	37.177	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	74.360%
24) Chloroform-d	4.253	84	57622	4.151	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.000%
26) 1,2-Dichloroethane-d4	4.947	65	27377	4.220	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.400%
32) Benzene-d6	4.960	84	115133	4.186	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.800%
36) 1,2-Dichloropropane-d6	5.989	67	32245	4.194	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.800%
41) Toluene-d8	7.243	98	105986	4.193	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.800%
43) trans-1,3-Dichloroprop...	7.561	79	11440	3.941	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.800%
46) 2-Hexanone-d5	8.027	63	36042	34.781	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	69.560%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	18281	3.922	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	78.400%
66) 1,2-Dichlorobenzene-d4	11.561	152	35738	4.216	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	84.400%
Target Compounds					Qvalue	
13) Acetone	2.130	43	4708	4.837	ug/L	# 39


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020524\
Data File : VV033980.D
Acq On : 05 Feb 2024 11:58
Operator : SY/MD
Sample : P1289-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG7

Quant Time: Feb 06 05:12:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Feb 06 05:11:25 2024
Response via : Initial Calibration

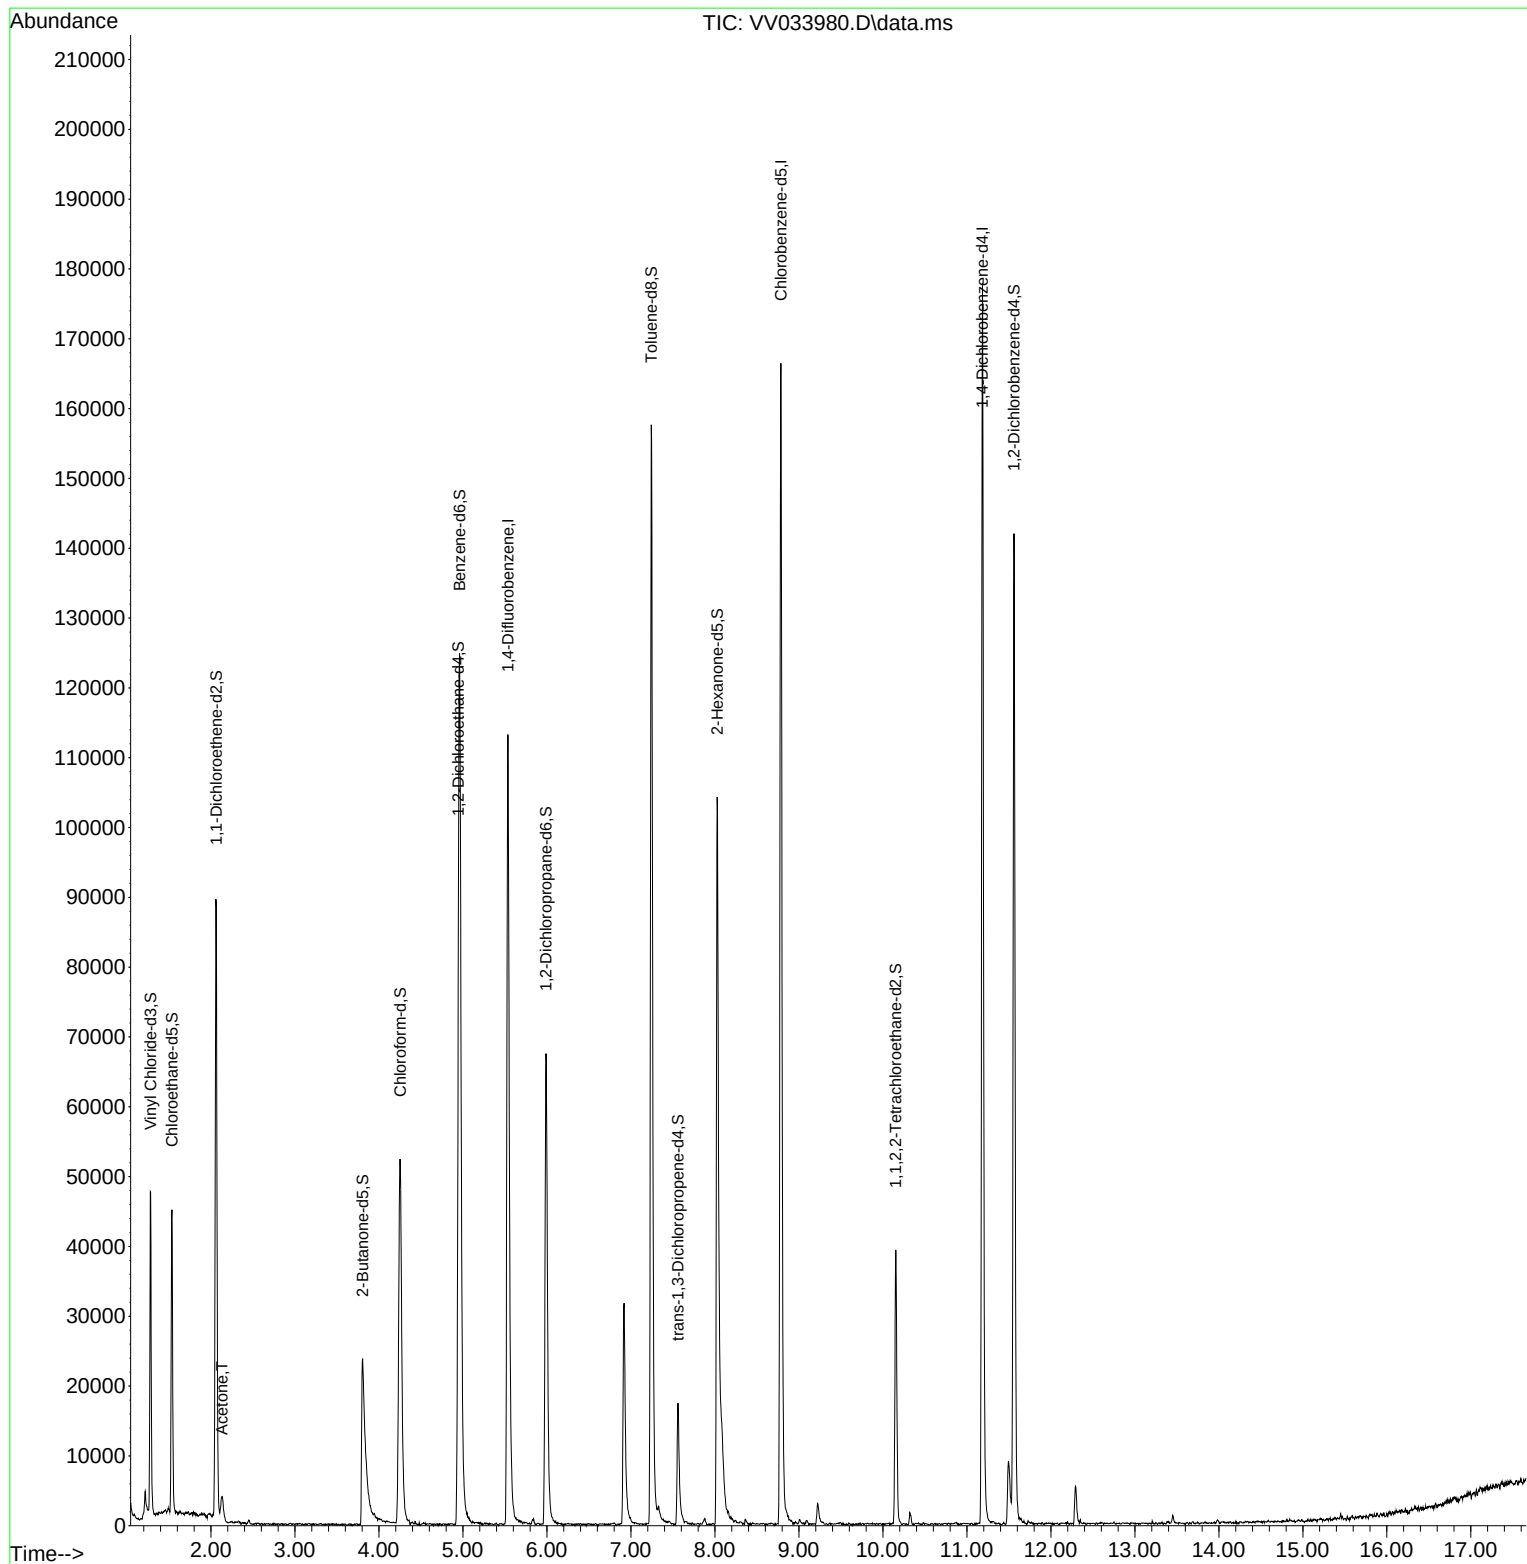

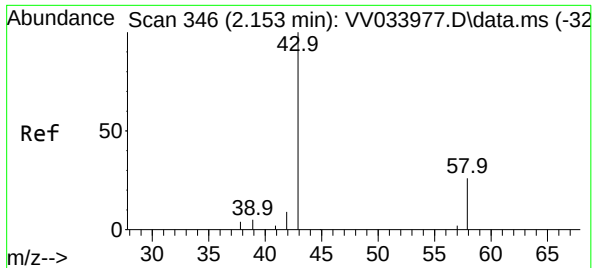

#13
Acetone
Concen: 4.837 ug/L
RT: 2.130 min Scan# 31
Delta R.T. -0.022 min
Lab File: VV033980.D
Acq: 05 Feb 2024 11:58

Instrument :
MSVOA_V
ClientSampleId :
C0AG7

Tgt Ion: 43 Resp: 4708
Ion Ratio Lower Upper
43 100
58 28.0 0.0 13.8#

