

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020524\
 Data File : VV033999.D
 Acq On : 05 Feb 2024 19:38
 Operator : SY/MD
 Sample : VIBLK318
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK318

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV033999.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	39902	43209	14.27%	1.545%
2	1.536	146	154	165	rVB	33235	38825	12.82%	1.388%
3	2.063	307	318	334	rBV2	76459	121993	40.29%	4.362%
4	2.452	431	439	450	rVB2	6386	10725	3.54%	0.384%
5	3.812	853	862	888	rBV	24508	77471	25.58%	2.770%
6	4.256	984	1000	1026	rBV	50405	130211	43.00%	4.656%
7	4.516	1064	1081	1110	rBV3	87345	230173	76.01%	8.231%
8	4.963	1205	1220	1246	rBV2	119725	302818	100.00%	10.828%
9	5.539	1388	1399	1424	rBV	107969	223633	73.85%	7.997%
10	5.992	1528	1540	1566	rBV	65988	140361	46.35%	5.019%
11	6.921	1819	1829	1852	rBV	29945	60128	19.86%	2.150%
12	7.246	1919	1930	1958	rBV	151467	272758	90.07%	9.753%
13	7.561	2019	2028	2053	rBV2	16218	31671	10.46%	1.133%
14	7.876	2116	2126	2136	rBV4	2059	3471	1.15%	0.124%
15	8.027	2164	2173	2212	rBV	131517	264865	87.47%	9.471%
16	8.786	2399	2409	2436	rBV	164268	277245	91.55%	9.914%
17	10.156	2825	2835	2856	rBV	43618	69619	22.99%	2.489%
18	11.188	3146	3156	3173	rBV	173668	271230	89.57%	9.699%
19	11.561	3262	3272	3298	rBV	140435	226130	74.68%	8.086%




Sum of corrected areas: 2796536

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020524\
Data File : VV033999.D
Acq On : 05 Feb 2024 19:38
Operator : SY/MD
Sample : VIBLK318
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

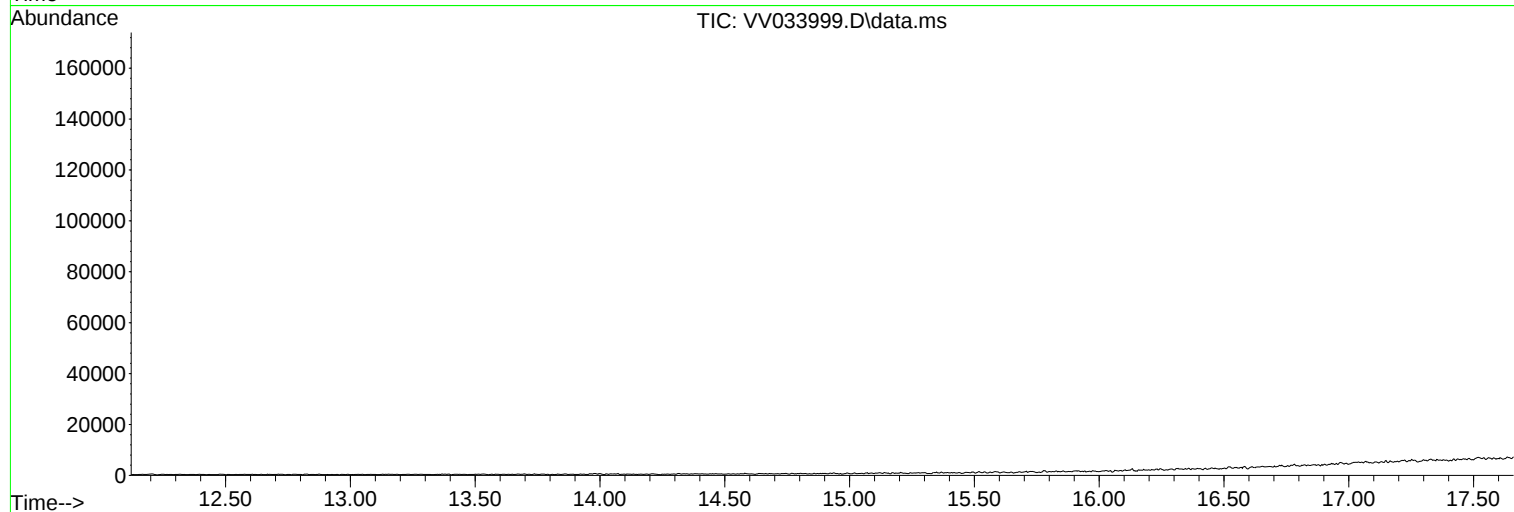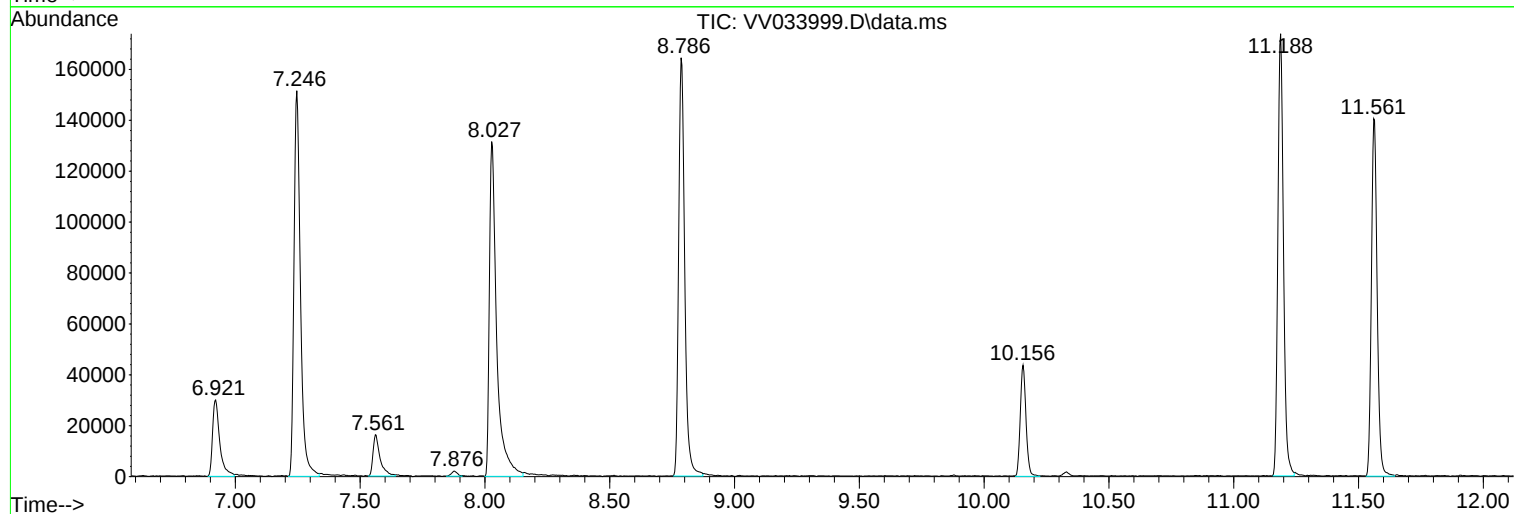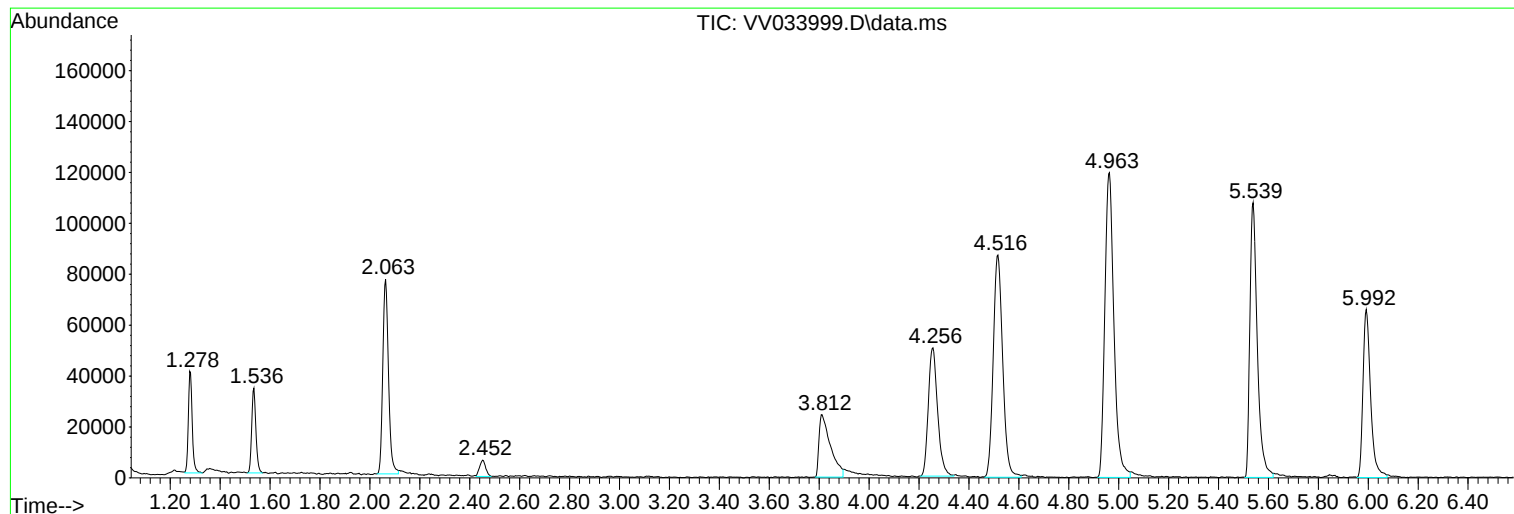

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020524\
Data File : VV033999.D
Acq On : 05 Feb 2024 19:38
Operator : SY/MD
Sample : VIBLK318
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020524\
Data File : VV033999.D
Acq On : 05 Feb 2024 19:38
Operator : SY/MD
Sample : VIBLK318
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
