


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020524\
Data File : VV033976.D
Acq On : 05 Feb 2024 08:45
Operator : SY/MD
Sample : BFB245
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB245

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Feb 08 04:46:29 2024

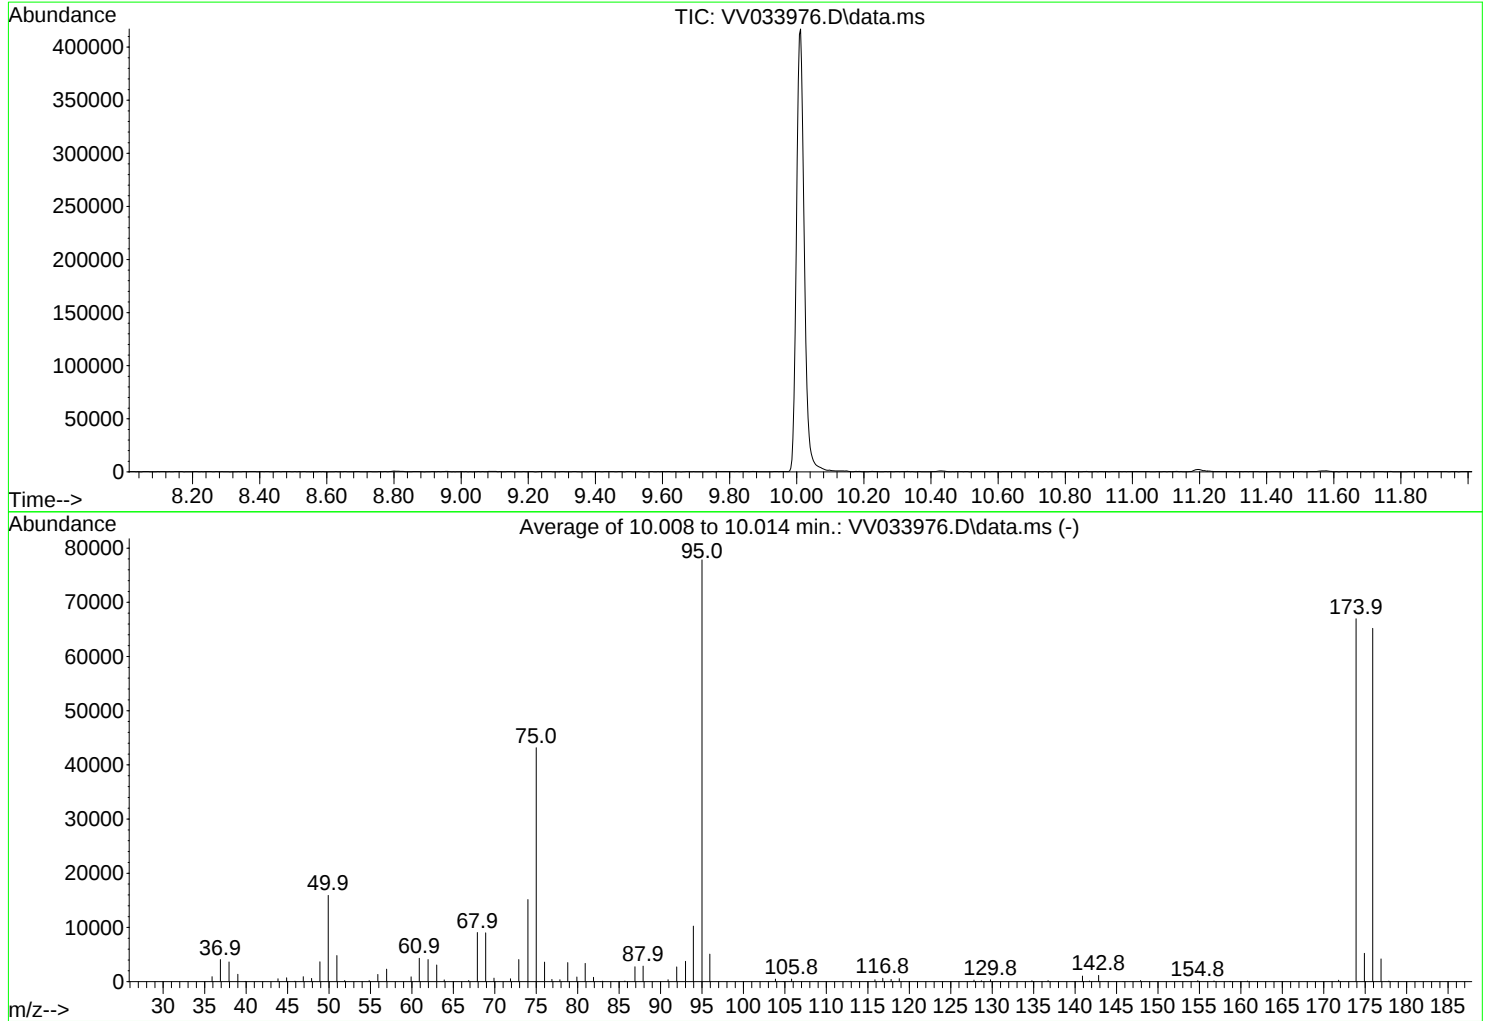

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	15923	PASS
75	95	30	80	55.5	43168	PASS
95	95	100	100	100.0	77837	PASS
96	95	5	9	6.5	5086	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.0	66965	PASS
175	174	5	9	7.8	5243	PASS
176	174	95	105	97.4	65208	PASS
177	176	5	10	6.4	4199	PASS

m/z	Abundance
40.00	118.0
43.70	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245

m/z	Abundance
35.90	961.0
36.90	4504.0
38.00	3877.0
39.00	1458.0
39.90	183.0
43.90	720.0
44.90	697.0
45.90	116.0
46.90	986.0
47.90	589.0
48.90	3832.0
49.90	16108.0
50.90	4960.0
51.90	232.0
54.90	231.0
55.90	1371.0
57.00	2457.0
59.90	945.0
60.90	4435.0
61.90	4136.0
63.00	3189.0
63.90	340.0
66.90	204.0
67.90	9638.0
68.90	9266.0
69.90	681.0
71.90	512.0
72.90	4136.0
74.00	15630.0
75.00	44624.0
76.00	3741.0
76.90	427.0
77.80	343.0
78.80	3581.0
79.90	824.0
80.90	3523.0
81.90	847.0
82.80	129.0
85.70	103.0
86.90	2815.0
87.90	3004.0
90.90	373.0
92.00	2615.0
93.00	3921.0
94.00	10395.0
95.00	79672.0
96.00	5103.0
103.80	491.0
104.80	105.0
105.80	491.0
112.90	103.0
115.80	368.0
116.80	650.0
117.80	413.0
118.80	596.0
127.80	295.0
128.70	169.0
129.80	380.0
134.80	165.0
136.80	224.0
140.00	101.0
140.90	998.0
141.70	128.0
142.90	1176.0
147.90	215.0
154.80	173.0
156.80	153.0
160.80	108.0
171.80	261.0
173.90	66888.0
174.90	5450.0
175.90	64864.0
176.90	4440.0
177.80	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245

m/z	Abundance
35.90	919.0
36.90	4140.0
38.00	3734.0
39.00	1423.0
39.80	196.0
43.90	681.0
44.90	757.0
45.90	123.0
46.90	949.0
47.90	620.0
48.90	3766.0
49.90	16400.0
51.00	4890.0
51.90	226.0
54.80	213.0
55.90	1392.0
57.00	2323.0
59.90	927.0
60.90	4437.0
62.00	4262.0
63.00	3162.0
63.90	345.0
66.90	230.0
67.90	9313.0
68.90	9272.0
69.90	682.0
71.90	560.0
72.90	4205.0
74.00	15530.0
75.00	44488.0
76.00	3721.0
76.90	398.0
77.80	362.0
78.80	3648.0
79.90	861.0
80.90	3480.0
81.90	817.0
83.00	121.0
85.70	119.0
86.90	2782.0
87.90	2918.0
90.90	352.0
92.00	2829.0
93.00	3862.0
94.00	10570.0
95.00	80320.0
95.90	5283.0
103.90	491.0
105.80	493.0
112.90	107.0
115.90	366.0
116.80	640.0
117.80	408.0
118.80	562.0
127.80	319.0
128.70	202.0
129.80	374.0
134.80	177.0
136.70	206.0
140.90	1092.0
141.80	127.0
142.90	1189.0
147.90	225.0
154.80	224.0
156.70	160.0
158.70	101.0
160.80	121.0
171.80	257.0
173.90	69360.0
174.90	5407.0
175.90	67384.0
176.90	4337.0
177.90	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245

m/z	Abundance
35.90	832.0
36.90	3552.0
37.90	3262.0
39.00	1186.0
39.80	189.0
43.90	575.0
44.90	716.0
46.90	825.0
47.90	606.0
48.90	3424.0
49.90	15261.0
51.00	4567.0
51.90	188.0
54.80	205.0
55.90	1276.0
56.90	2098.0
59.90	801.0
60.90	4088.0
62.00	3799.0
63.00	2888.0
63.90	314.0
66.80	233.0
67.90	8231.0
68.90	8505.0
69.90	630.0
71.90	543.0
72.90	3903.0
74.00	14259.0
75.00	40392.0
76.00	3332.0
76.90	383.0
77.90	360.0
78.80	3340.0
79.90	889.0
80.90	3135.0
81.90	715.0
83.00	114.0
85.70	111.0
86.90	2665.0
87.90	2643.0
90.90	342.0
91.90	2693.0
93.00	3457.0
93.90	9748.0
95.00	73520.0
95.90	4871.0
103.90	446.0
105.80	453.0
115.90	339.0
116.80	586.0
117.80	381.0
118.80	515.0
127.80	303.0
128.70	192.0
129.80	329.0
134.80	158.0
136.80	161.0
140.90	1014.0
141.80	101.0
142.80	1098.0
145.80	119.0
147.90	198.0
154.80	206.0
156.70	141.0
158.70	108.0
160.80	133.0
171.80	248.0
173.90	64648.0
174.90	4873.0
175.90	63376.0
176.90	3819.0
177.90	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245