

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020525\
 Data File : VV038620.D
 Acq On : 05 Feb 2025 10:37
 Operator : SY/MD
 Sample : VV0205WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Feb 06 07:32:45 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 28 08:06:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	3868	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	3997	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	1839	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	2141	0.549	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery = 110.000%			
4) 1,2-Dichloroethane-d4	4.969	65	1772	0.569	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 114.000%			
7) 1,2-Dichloropropane-d6	5.995	67	2205	0.561	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery = 112.000%			
8) Toluene-d8	7.253	98	4114	0.522	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 104.000%			
10) 1,1,2,2-Tetrachloroeth...	10.146	84	1909	0.570	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery = 114.000%			
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.339	75	8	0.024	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020525\
Data File : VV038620.D
Acq On : 05 Feb 2025 10:37
Operator : SY/MD
Sample : VV0205WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Feb 06 07:32:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 28 08:06:10 2025
Response via : Initial Calibration

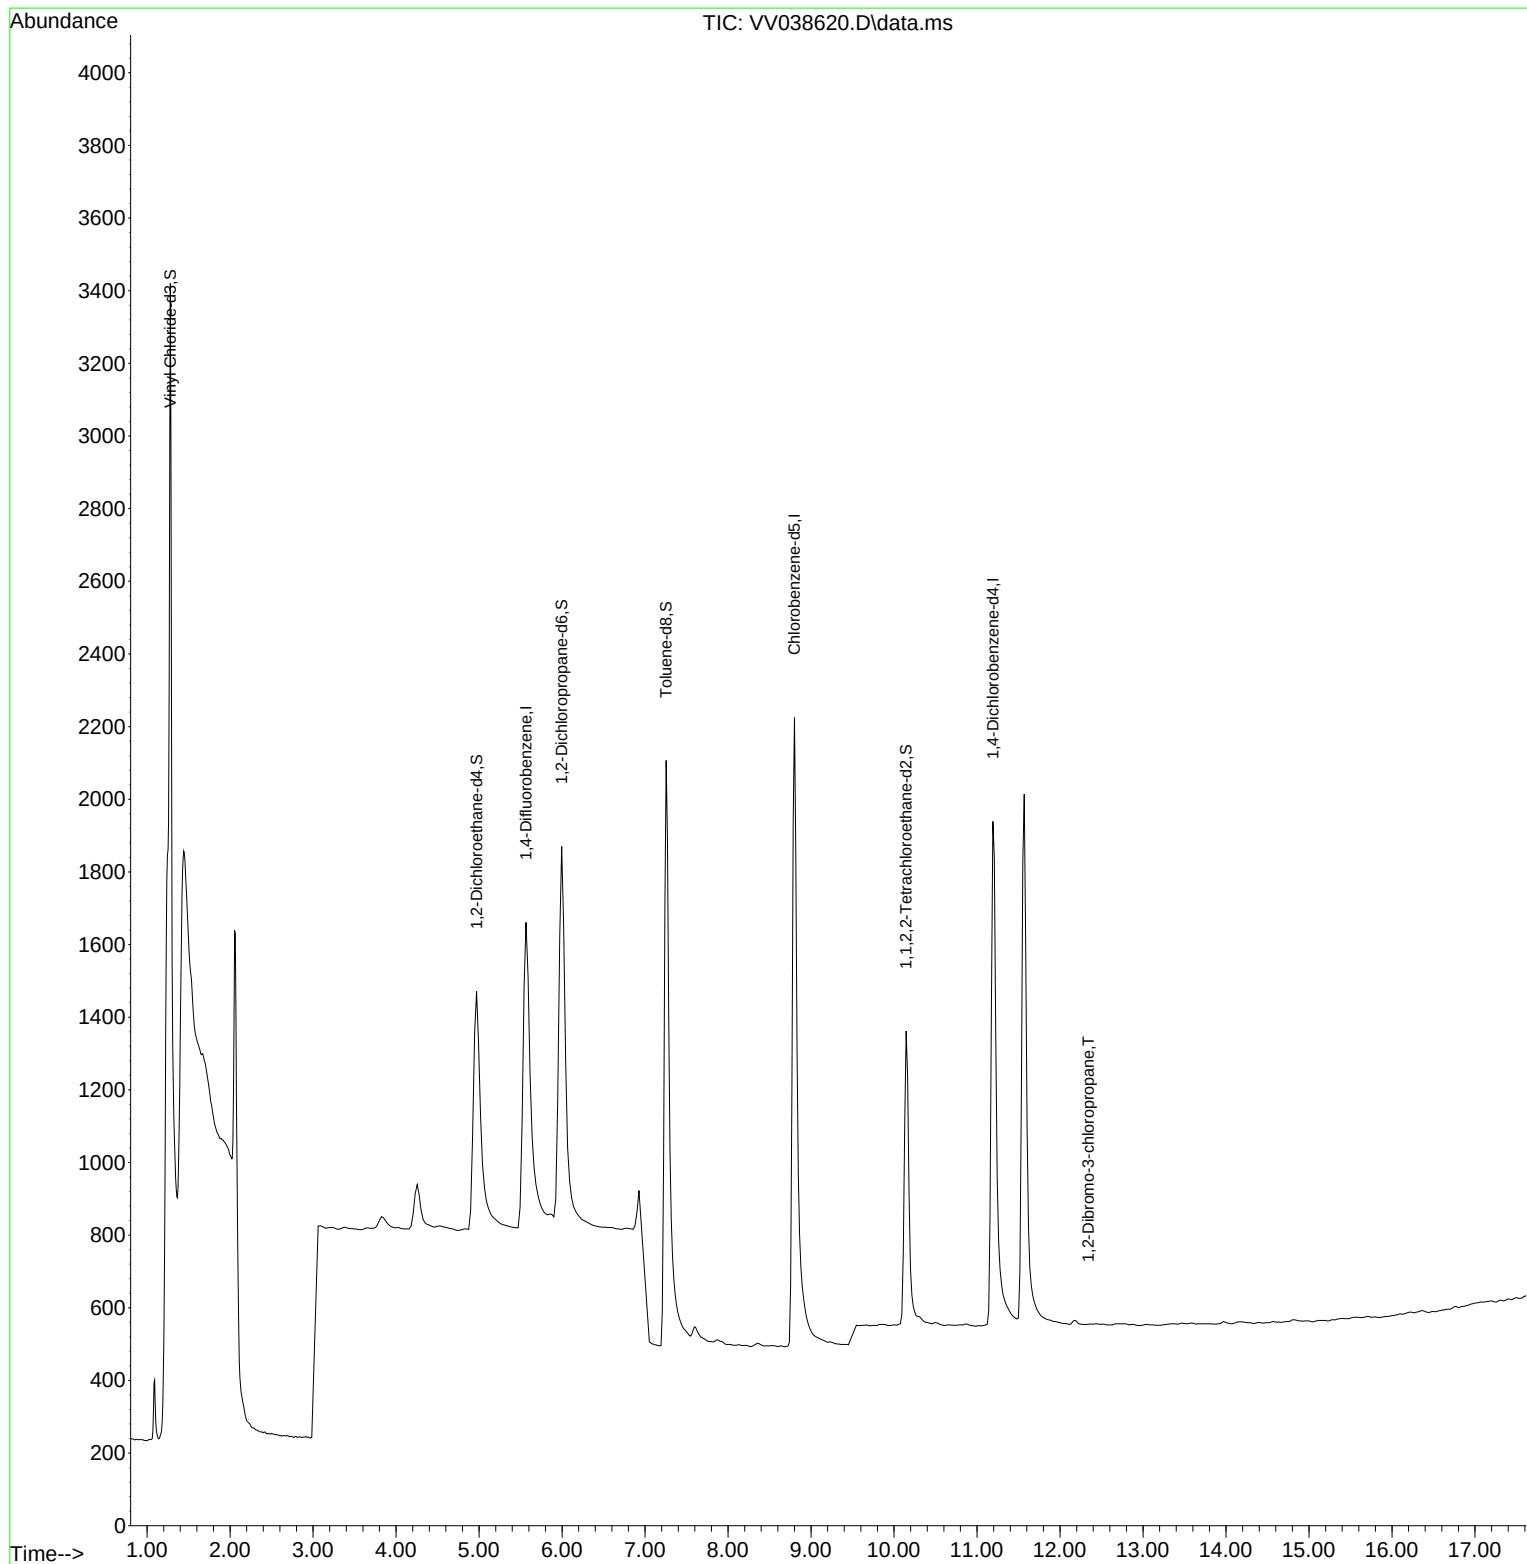

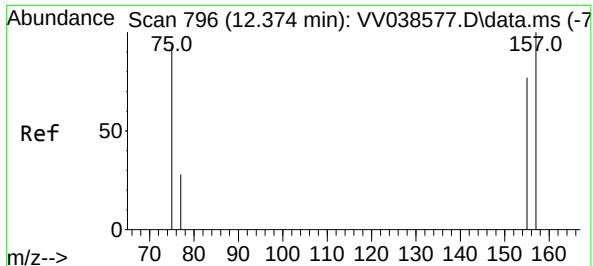

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.024 ug/L
 RT: 12.339 min Scan# 79
 Delta R.T. -0.034 min
 Lab File: VV038620.D
 Acq: 05 Feb 2025 10:37

Instrument :
 MSVOA_V
 ClientSampleId :

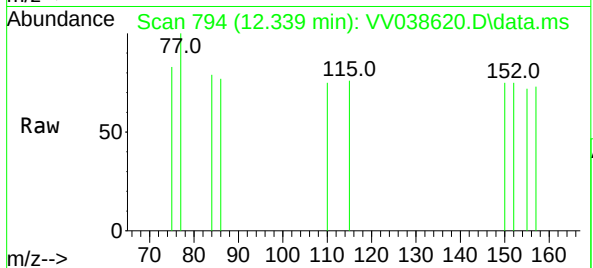

Tgt Ion: 75	Resp:	8	
Ion Ratio	Lower	Upper	
75 100			
157	88.1	77.0	115.6
155	86.4	68.2	102.2

