

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020525\
 Data File : VV038629.D
 Acq On : 05 Feb 2025 16:11
 Operator : SY/MD
 Sample : Q1226-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Feb 06 07:33:29 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 28 08:06:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	5072	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	5026	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	2360	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	2021	0.395	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	80.000%		
4) 1,2-Dichloroethane-d4	4.969	65	1734	0.425	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	84.000%		
7) 1,2-Dichloropropane-d6	5.995	67	2102	0.425	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	86.000%		
8) Toluene-d8	7.253	98	3865	0.390	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	78.000%		
10) 1,1,2,2-Tetrachloroeth...	10.146	84	1941	0.461	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	92.000%		
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.168	75	39	0.092	ug/L	Qvalue # 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020525\
Data File : VV038629.D
Acq On : 05 Feb 2025 16:11
Operator : SY/MD
Sample : Q1226-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Feb 06 07:33:29 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 28 08:06:10 2025
Response via : Initial Calibration

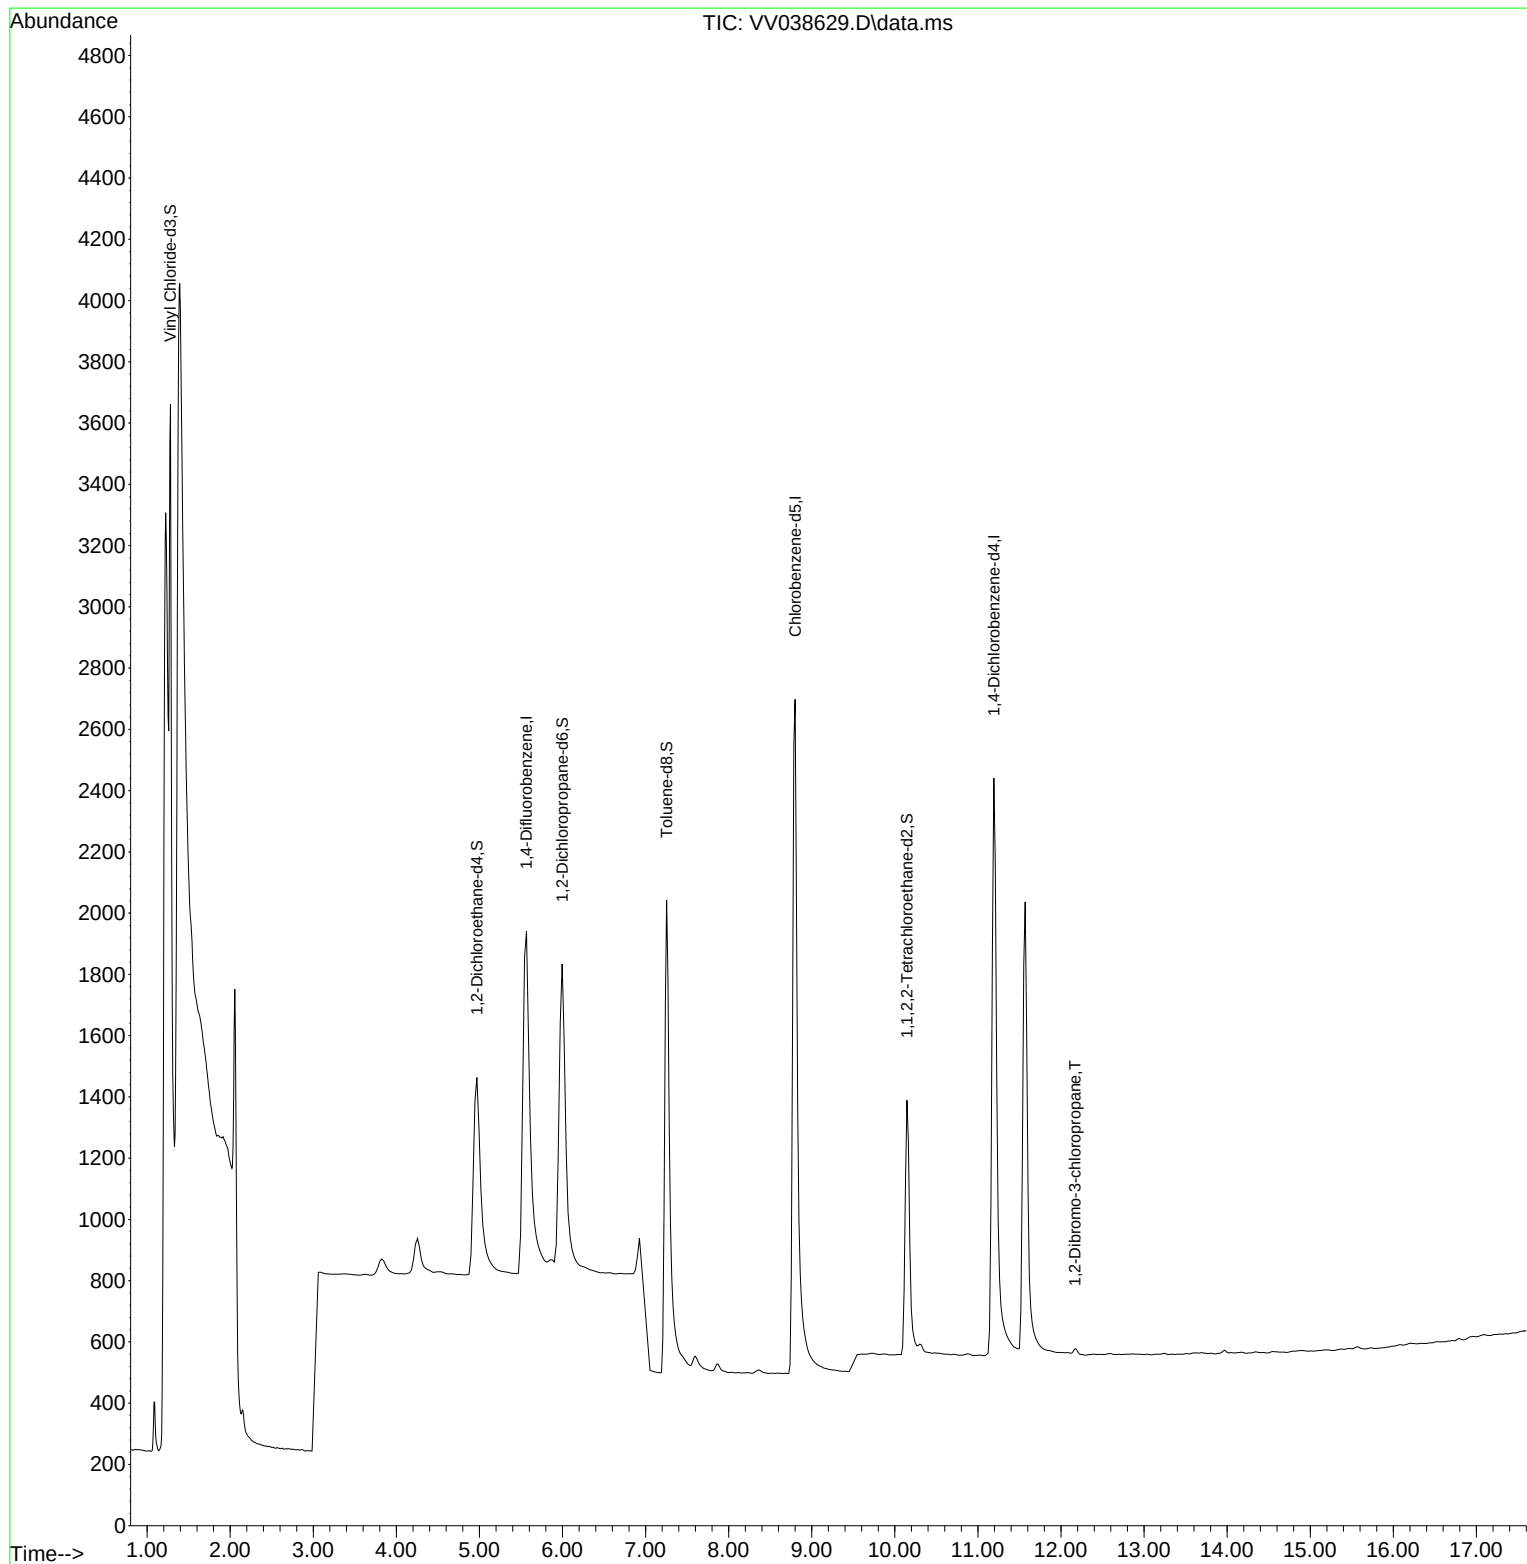

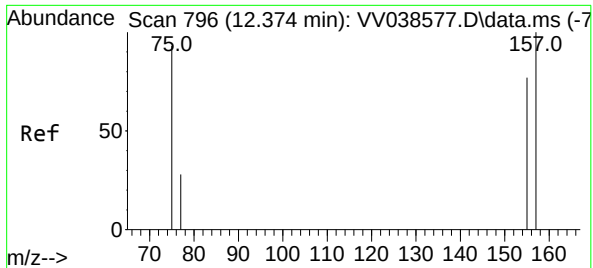

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.092 ug/L
 RT: 12.168 min Scan# 71
 Delta R.T. -0.206 min
 Lab File: VV038629.D
 Acq: 05 Feb 2025 16:11

Instrument :
 MSVOA_V
 ClientSampleId :

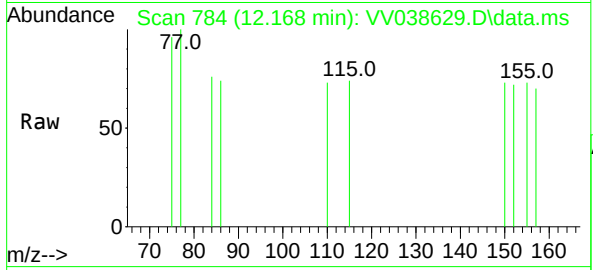

Tgt Ion: 75	Resp:	39
Ion	Ratio	Lower Upper
75	100	
157	73.2	77.0 115.6#
155	76.1	68.2 102.2

