

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020525\
 Data File : VV038622.D
 Acq On : 05 Feb 2025 11:45
 Operator : SY/MD
 Sample : Q1226-13DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZN3DL

Quant Time: Feb 06 07:32:56 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 28 08:06:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	5681	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	5726	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	2614	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	2309	0.403	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	80.000%
4) 1,2-Dichloroethane-d4	4.969	65	1968	0.430	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	86.000%
7) 1,2-Dichloropropane-d6	5.995	67	2388	0.424	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	84.000%
8) Toluene-d8	7.253	98	4513	0.400	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	80.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2137	0.445	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	90.000%
Target Compounds						
6) Trichloroethene	5.852	95	2780	0.588	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020525\
Data File : VV038622.D
Acq On : 05 Feb 2025 11:45
Operator : SY/MD
Sample : Q1226-13DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCZN3DL


Quant Time: Feb 06 07:32:56 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 28 08:06:10 2025
Response via : Initial Calibration

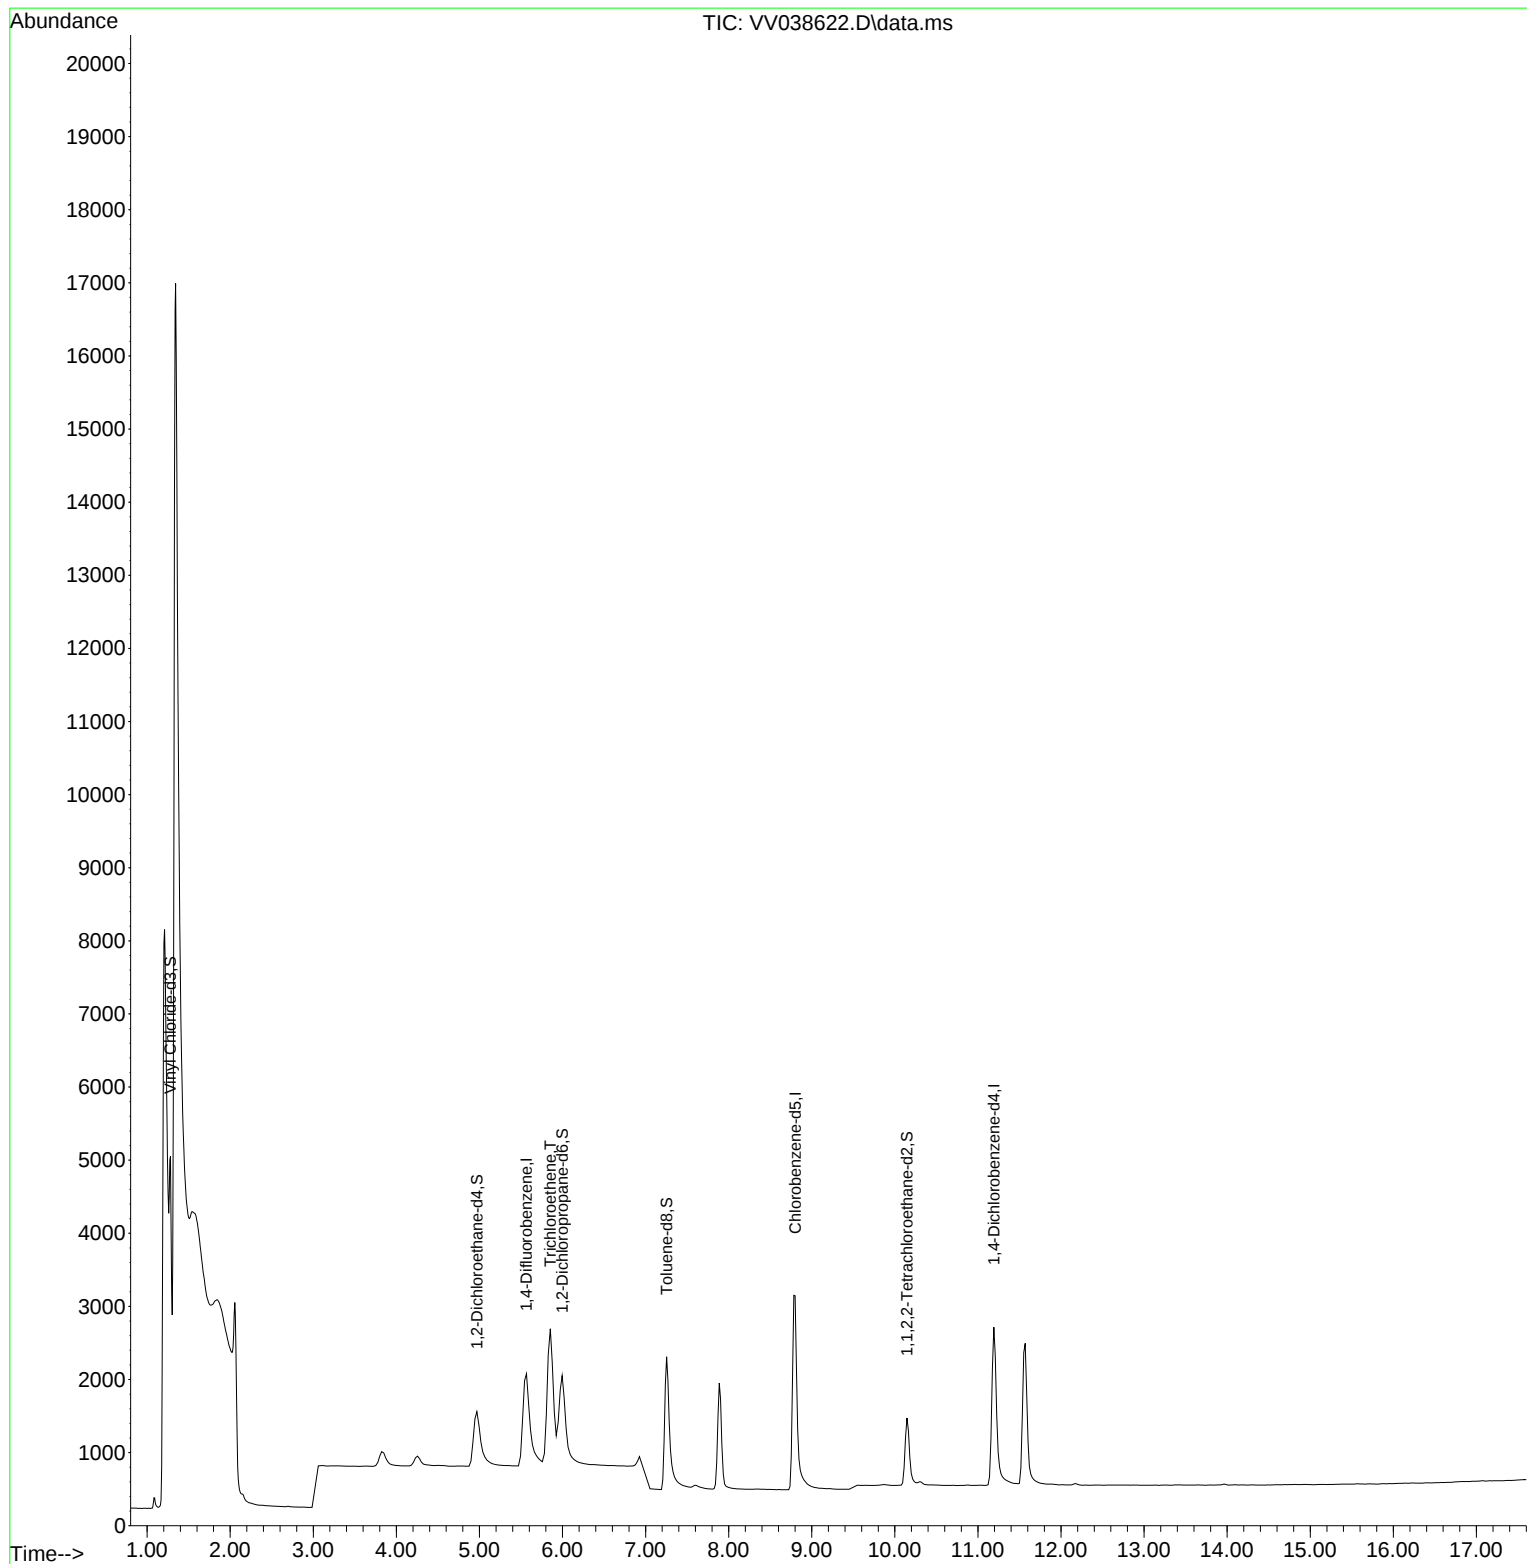

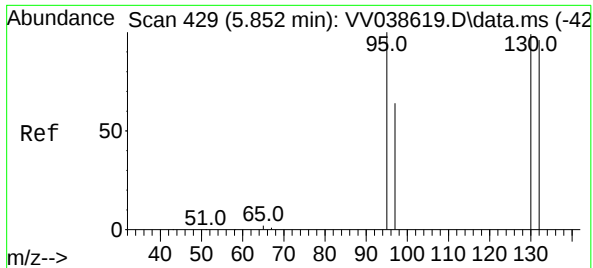

Trichloroethene
 Concen: 0.588 ug/L
 RT: 5.852 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: VV038622.D
 Acq: 05 Feb 2025 11:45

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZN3DL

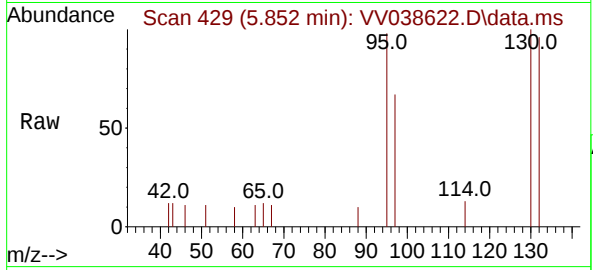

Tgt Ion: 95	Resp:	2780
Ion	Ratio	Lower Upper
95	100	
97	67.9	47.9 88.9
132	97.3	68.2 126.6
130	101.6	69.7 129.5

