

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV020525\  
 Data File : VV038626.D  
 Acq On : 05 Feb 2025 14:46  
 Operator : SY/MD  
 Sample : Q1226-17DL 10X  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 DCZN8DL

Quant Time: Feb 06 07:33:15 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVSIM012725.M  
 Quant Title : TRACE VOA SOM01.0  
 QLast Update : Tue Jan 28 08:06:10 2025  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response   | Conc    | Units | Dev(Min)  |
|-------------------------------|----------------|------|------------|---------|-------|-----------|
| -----                         |                |      |            |         |       |           |
| Internal Standards            |                |      |            |         |       |           |
| 1) 1,4-Difluorobenzene        | 5.566          | 114  | 5320       | 0.500   | ug/L  | 0.00      |
| 5) Chlorobenzene-d5           | 8.800          | 117  | 5413       | 0.500   | ug/L  | 0.00      |
| 11) 1,4-Dichlorobenzene-d4    | 11.191         | 152  | 2513       | 0.500   | ug/L  | 0.00      |
| System Monitoring Compounds   |                |      |            |         |       |           |
| 2) Vinyl Chloride-d3          | 1.280          | 65   | 2169       | 0.404   | ug/L  | 0.00      |
| Spiked Amount 0.500           | Range 40 - 130 |      | Recovery = | 80.000% |       |           |
| 4) 1,2-Dichloroethane-d4      | 4.969          | 65   | 1847       | 0.431   | ug/L  | 0.00      |
| Spiked Amount 0.500           | Range 70 - 130 |      | Recovery = | 86.000% |       |           |
| 7) 1,2-Dichloropropane-d6     | 5.995          | 67   | 2262       | 0.425   | ug/L  | 0.00      |
| Spiked Amount 0.500           | Range 60 - 140 |      | Recovery = | 86.000% |       |           |
| 8) Toluene-d8                 | 7.253          | 98   | 4217       | 0.395   | ug/L  | 0.00      |
| Spiked Amount 0.500           | Range 70 - 130 |      | Recovery = | 80.000% |       |           |
| 10) 1,1,2,2-Tetrachloroeth... | 10.146         | 84   | 2025       | 0.446   | ug/L  | 0.00      |
| Spiked Amount 0.500           | Range 65 - 120 |      | Recovery = | 90.000% |       |           |
| Target Compounds              |                |      |            |         |       |           |
| 6) Trichloroethene            | 5.828          | 95   | 5121       | 1.145   | ug/L  | Qvalue 95 |
| -----                         |                |      |            |         |       |           |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV020525\  
Data File : VV038626.D  
Acq On : 05 Feb 2025 14:46  
Operator : SY/MD  
Sample : Q1226-17DL 10X  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
DCZN8DL

Quant Time: Feb 06 07:33:15 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVSIM012725.M  
Quant Title : TRACE VOA SOM01.0  
QLast Update : Tue Jan 28 08:06:10 2025  
Response via : Initial Calibration

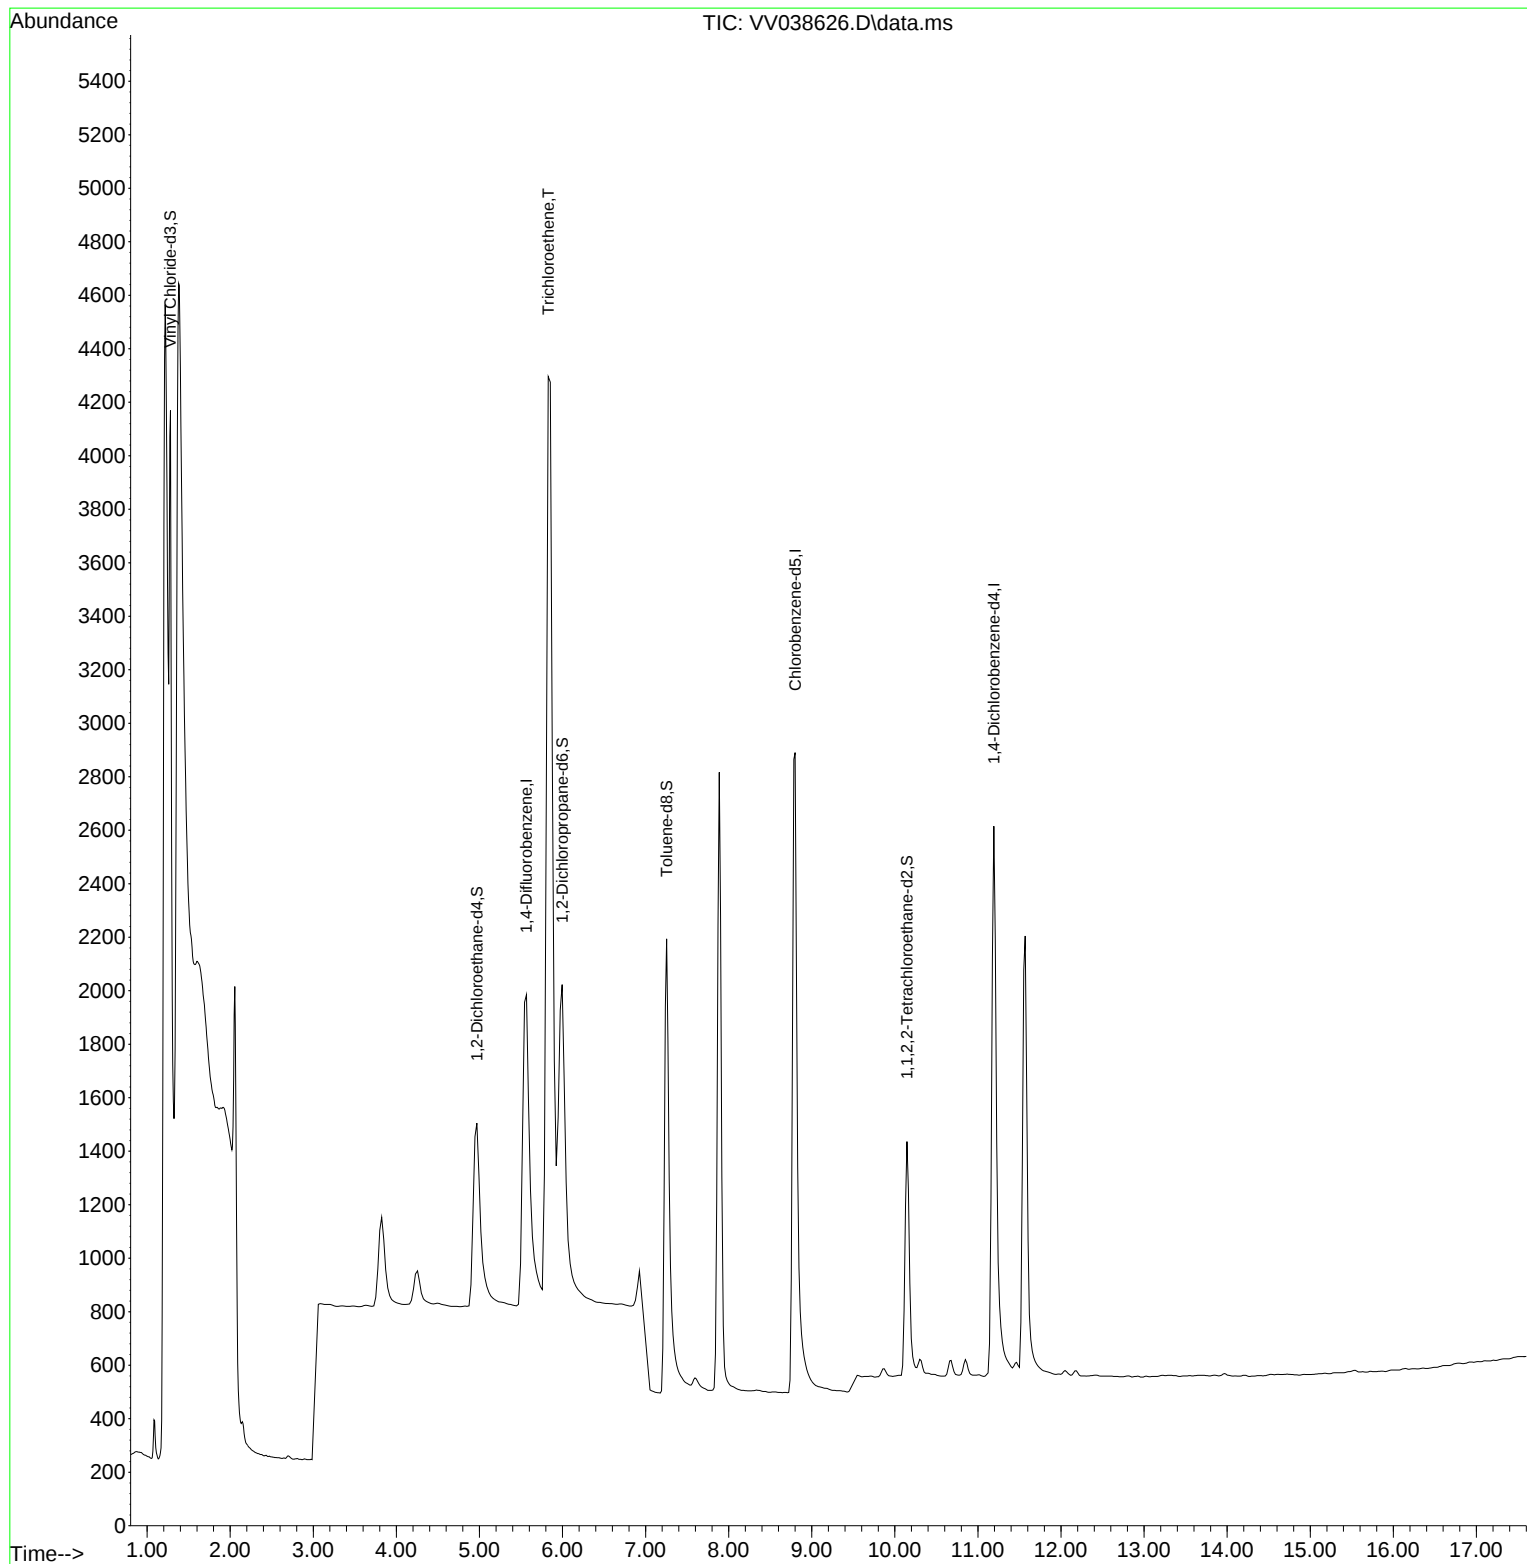

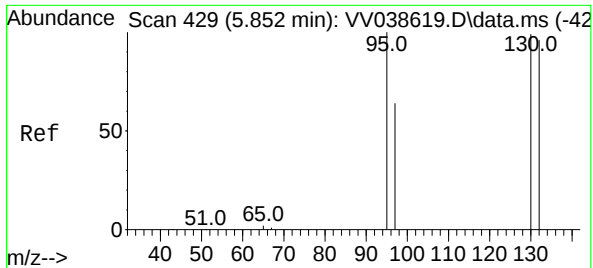

Trichloroethene

Concen: 1.145 ug/L

RT: 5.828 min Scan# 41

Delta R.T. -0.024 min

Lab File: VV038626.D


Acq: 05 Feb 2025 14:46

Instrument :

MSVOA\_V

ClientSampleId :

DCZN8DL

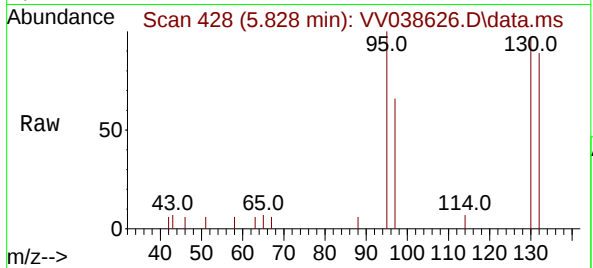

Tgt Ion: 95 Resp: 5121

Ion Ratio Lower Upper

95 100

97 66.4 47.9 88.9

132 89.1 68.2 126.6

130 96.9 69.7 129.5

