

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020525\
 Data File : VV038627.D
 Acq On : 05 Feb 2025 15:10
 Operator : SY/MD
 Sample : Q1226-22DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZL9DL

Quant Time: Feb 06 07:33:20 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 28 08:06:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	4119	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	4297	0.500	ug/L	-0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	2045	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	1357	0.327	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	66.000%		
4) 1,2-Dichloroethane-d4	4.969	65	1500	0.452	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	90.000%		
7) 1,2-Dichloropropane-d6	5.995	67	1728	0.409	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	82.000%		
8) Toluene-d8	7.253	98	2994	0.354	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	70.000%		
10) 1,1,2,2-Tetrachloroeth...	10.146	84	1793	0.498	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	100.000%		
Target Compounds						
6) Trichloroethene	5.852	95	2102	0.592	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020525\
Data File : VV038627.D
Acq On : 05 Feb 2025 15:10
Operator : SY/MD
Sample : Q1226-22DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCZL9DL

Quant Time: Feb 06 07:33:20 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 28 08:06:10 2025
Response via : Initial Calibration

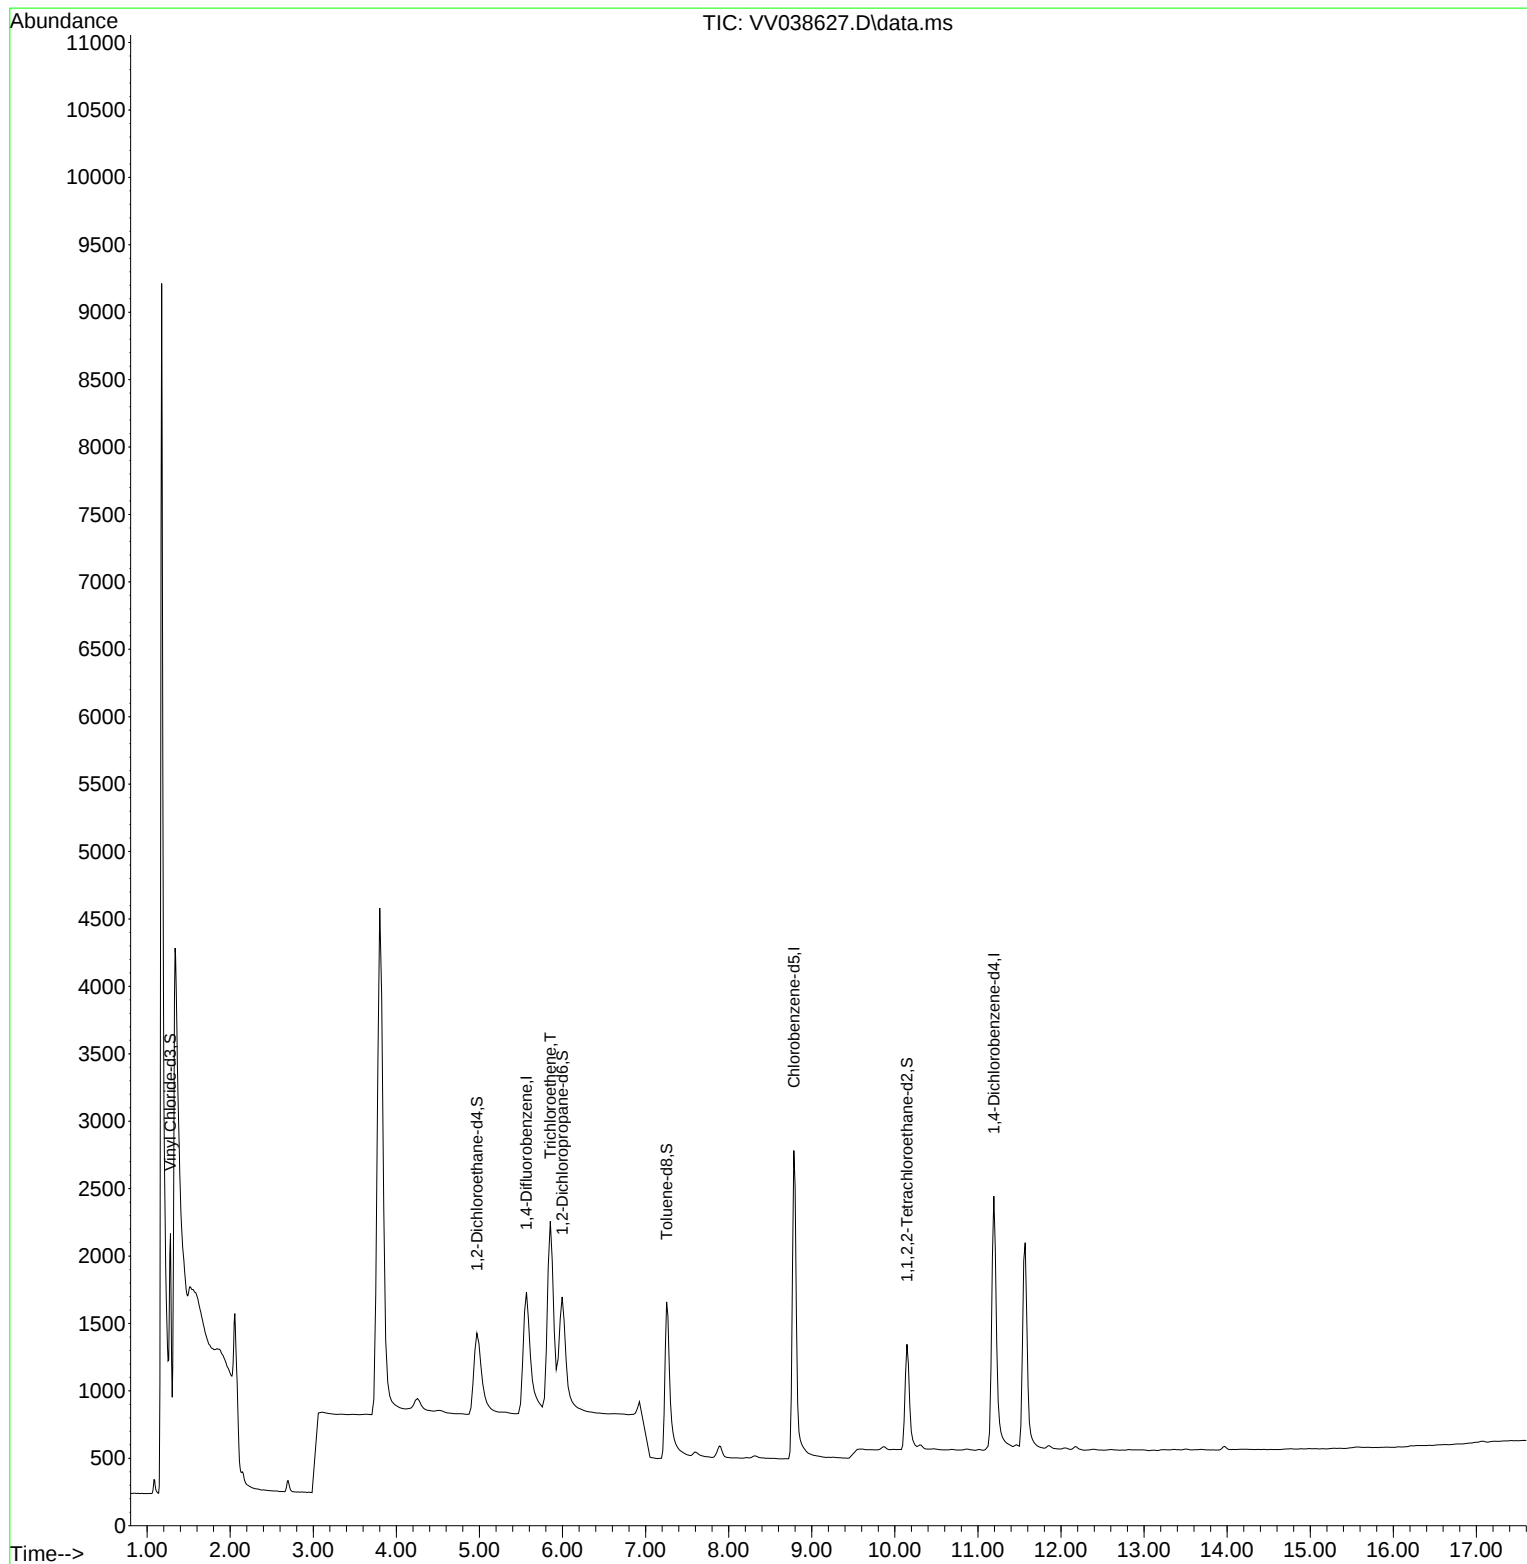

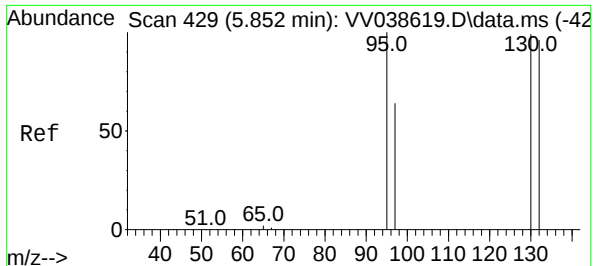

Trichloroethene

Concen: 0.592 ug/L

RT: 5.852 min Scan# 41

Delta R.T. 0.000 min

Lab File: VV038627.D


Acq: 05 Feb 2025 15:10

Instrument :

MSVOA_V

ClientSampleId :

DCZL9DL

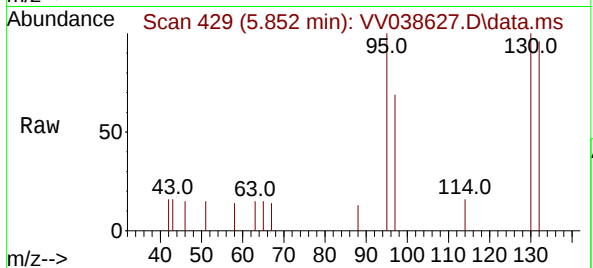

Tgt Ion: 95 Resp: 2102

Ion Ratio Lower Upper

95 100

97 68.9 47.9 88.9

132 96.4 68.2 126.6

130 99.5 69.7 129.5

