

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020525\
 Data File : VV038628.D
 Acq On : 05 Feb 2025 15:35
 Operator : SY/MD
 Sample : Q1226-23DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCZN9DL

Quant Time: Feb 06 07:33:25 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jan 28 08:06:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	6496	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	6323	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	2878	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	2147	0.328	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	66.000%		
4) 1,2-Dichloroethane-d4	4.969	65	2077	0.397	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	80.000%		
7) 1,2-Dichloropropane-d6	5.995	67	2480	0.399	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	80.000%		
8) Toluene-d8	7.253	98	4734	0.380	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	76.000%		
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2204	0.416	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	84.000%		
Target Compounds						
6) Trichloroethene	5.852	95	2961	0.567	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020525\
Data File : VV038628.D
Acq On : 05 Feb 2025 15:35
Operator : SY/MD
Sample : Q1226-23DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCZN9DL

Quant Time: Feb 06 07:33:25 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jan 28 08:06:10 2025
Response via : Initial Calibration

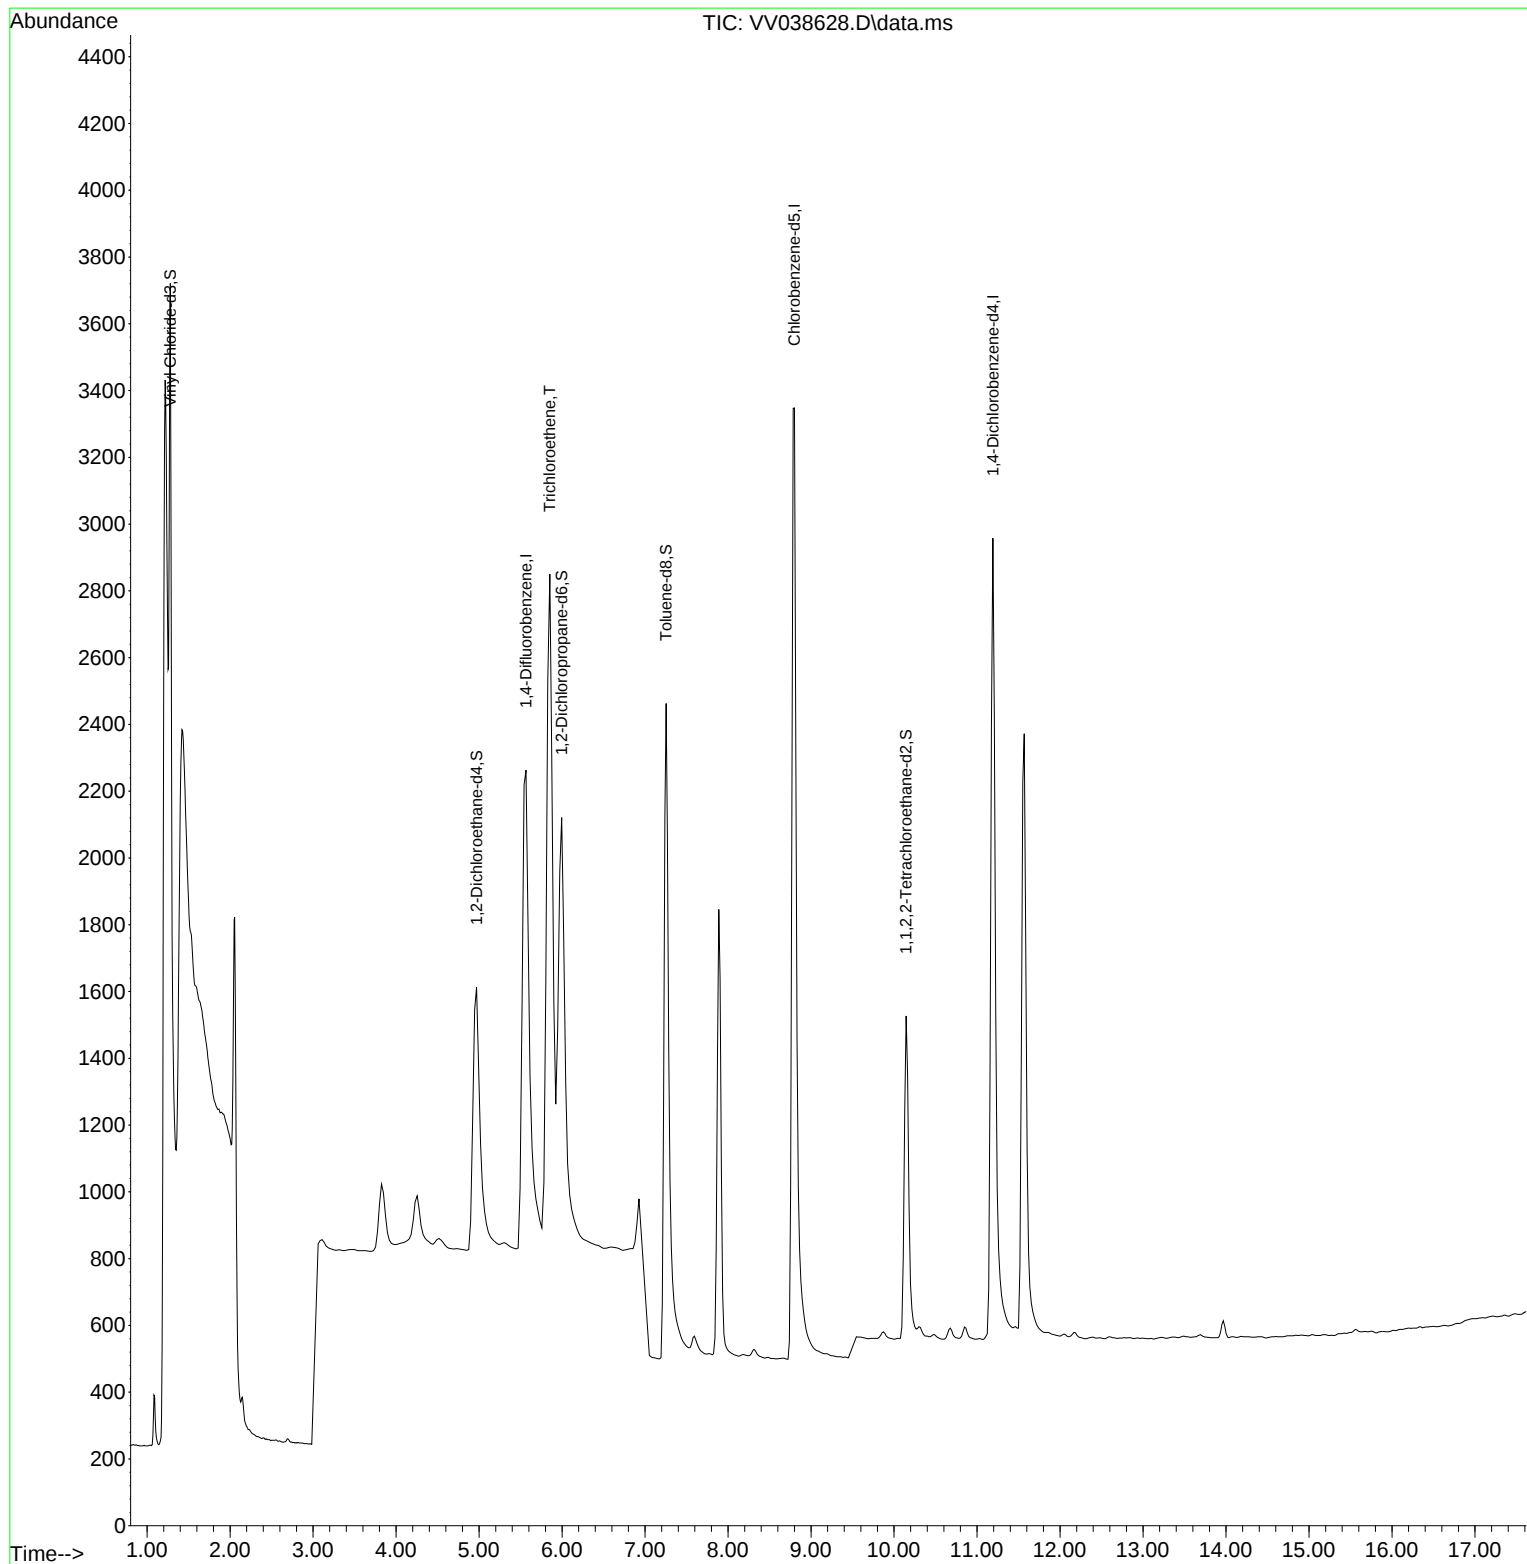

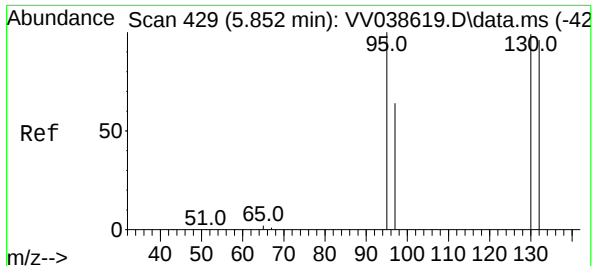

Trichloroethene

Concen: 0.567 ug/L

RT: 5.852 min Scan# 41

Delta R.T. 0.000 min

Lab File: VV038628.D


Acq: 05 Feb 2025 15:35

Instrument :

MSVOA_V

ClientSampleId :

DCZN9DL

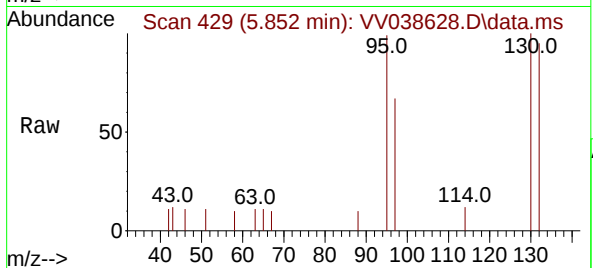

Tgt Ion: 95 Resp: 2961

Ion Ratio Lower Upper

95 100

97 67.7 47.9 88.9

132 96.3 68.2 126.6

130 101.2 69.7 129.5

