


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020525\
Data File : VV038618.D
Acq On : 05 Feb 2025 08:34
Operator : SY/MD
Sample : BFB232
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB232

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM012725.M
Title : TRACE VOA SOM01.0
Last Update : Tue Jan 28 08:06:10 2025

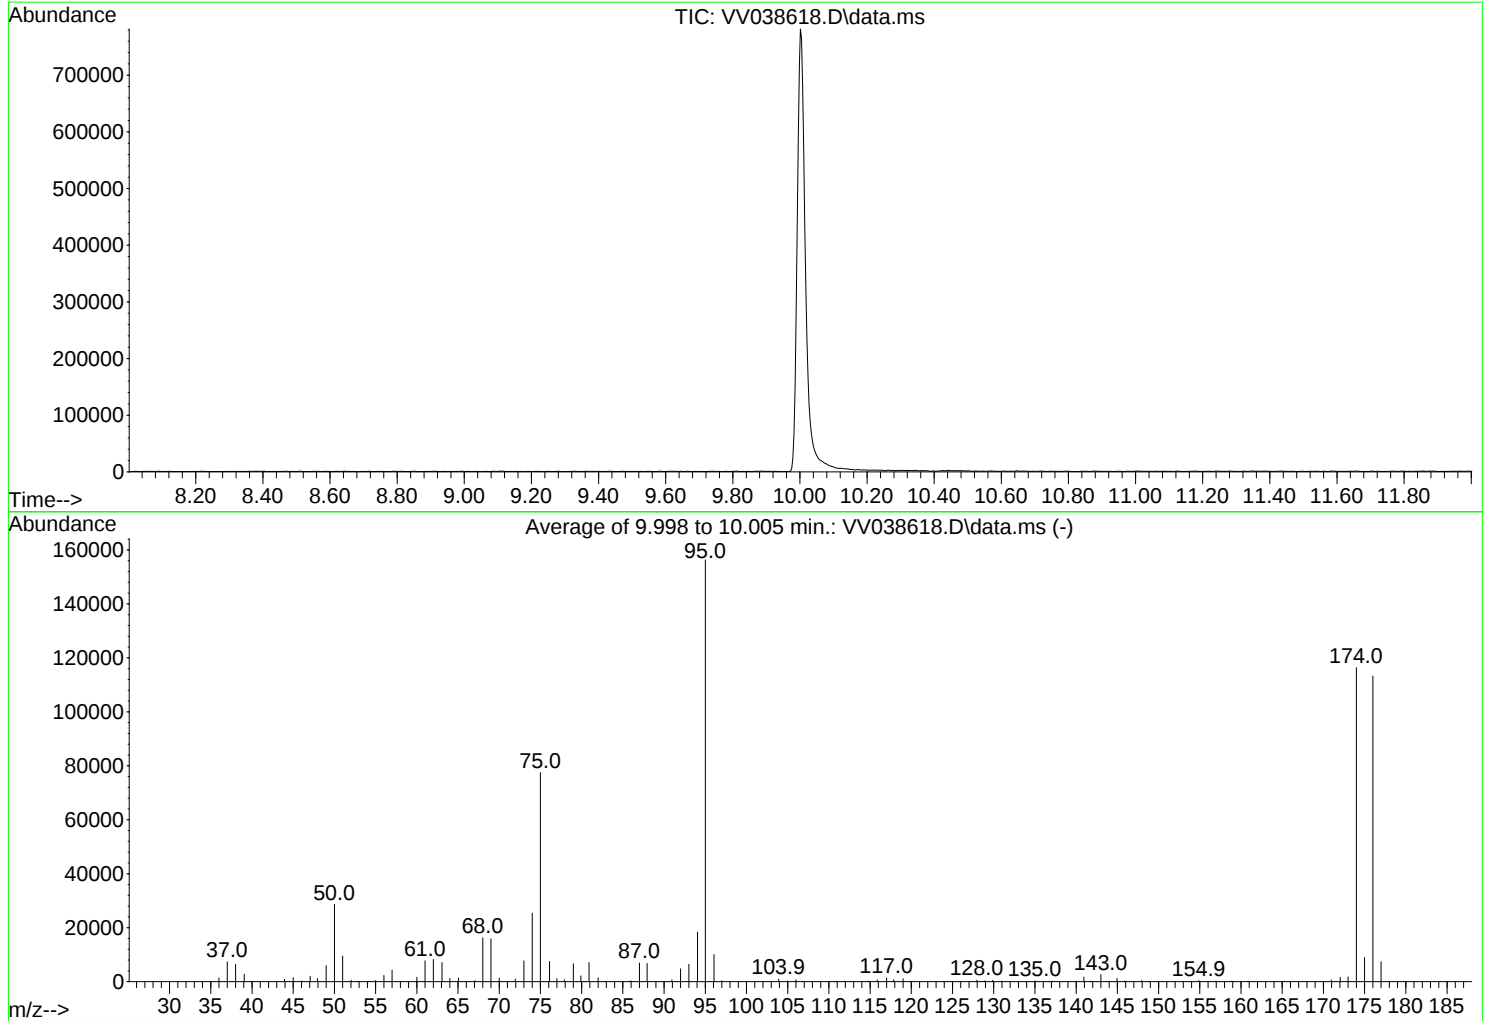

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2774

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.3	28621	PASS
75	95	30	80	49.6	77528	PASS
95	95	100	100	100.0	156331	PASS
96	95	5	9	6.4	10007	PASS
173	174	0.00	2	1.5	1774	PASS
174	95	50	120	74.4	116376	PASS
175	174	5	9	7.7	8984	PASS
176	174	95	101	97.3	113240	PASS
177	176	5	9	6.6	7443	PASS

m/z	Abundance
40.00	222.0
43.90	399.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

m/z	Abundance
35.10	106.0
36.00	1321.0
37.00	7086.0
38.00	6302.0
39.10	2895.0
40.00	424.0
42.90	126.0
44.00	1238.0
45.00	1423.0
46.10	350.0
47.00	2134.0
47.90	1213.0
49.00	5815.0
50.00	27344.0
51.00	9197.0
52.10	512.0
52.80	236.0
55.00	476.0
56.00	2267.0
57.00	4125.0
58.10	198.0
60.00	1570.0
61.00	7706.0
62.00	8012.0
63.10	6823.0
64.00	1195.0
65.10	1269.0
66.00	201.0
67.10	392.0
68.00	15641.0
69.00	15144.0
70.00	1308.0
72.00	914.0
73.00	7425.0
74.00	24544.0
75.00	74168.0
76.10	7373.0
77.00	1184.0
77.90	706.0
79.00	6427.0
79.90	2066.0
80.90	6846.0
82.00	1414.0
82.80	114.0
85.80	289.0
86.10	291.0
87.00	6674.0
87.90	6762.0
91.00	665.0
92.00	4669.0
93.00	6066.0
94.00	17368.0
95.00	148736.0
96.00	9927.0
97.00	369.0
103.90	846.0
104.90	280.0
106.00	618.0
106.70	131.0
110.90	147.0
111.10	150.0
111.90	110.0
113.00	204.0
114.80	178.0
115.90	634.0
117.00	1257.0
117.80	647.0
119.00	1007.0
124.00	108.0
128.00	497.0
128.90	320.0
129.90	490.0
130.90	216.0
135.00	314.0
136.70	199.0
137.20	210.0
140.00	144.0
140.90	1799.0
141.80	195.0
143.00	2551.0
144.00	212.0
144.90	1100.0
145.90	272.0
148.00	312.0
148.90	134.0
149.90	120.0
151.70	115.0
153.00	123.0
153.90	146.0
154.90	430.0
155.90	114.0
156.90	225.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

158.80	201.0
160.80	165.0
170.90	608.0
172.10	1373.0
173.00	1641.0
174.00	109408.0
175.00	8349.0
176.00	105216.0
177.00	7062.0
178.00	235.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

m/z	Abundance
36.00	1389.0
37.00	7665.0
38.00	6607.0
39.10	2784.0
40.00	358.0
43.00	120.0
44.00	1248.0
45.00	1559.0
46.10	286.0
47.00	2011.0
48.00	1224.0
49.00	6129.0
50.00	29600.0
51.00	9985.0
52.10	540.0
53.00	213.0
55.00	442.0
56.00	2352.0
57.00	4453.0
58.10	159.0
60.00	1663.0
61.00	7913.0
62.00	8673.0
63.00	7321.0
64.00	1267.0
65.10	1333.0
65.90	211.0
67.00	434.0
68.00	16896.0
69.00	16512.0
70.00	1354.0
71.90	963.0
73.00	8015.0
74.00	26288.0
75.00	80240.0
76.10	7807.0
77.00	1186.0
77.90	674.0
79.00	6805.0
79.90	2290.0
80.90	7294.0
82.00	1445.0
82.90	142.0
85.90	369.0
87.00	7246.0
88.00	7035.0
91.00	687.0
92.00	4850.0
93.00	6621.0
94.10	18888.0
95.00	162176.0
96.10	10192.0
97.00	404.0
103.90	969.0
105.00	323.0
106.00	707.0
106.80	141.0
107.90	132.0
110.10	120.0
110.90	191.0
111.90	169.0
113.00	229.0
114.70	184.0
115.80	713.0
117.00	1461.0
117.90	692.0
119.00	1087.0
123.90	120.0
128.00	565.0
128.90	341.0
129.80	464.0
130.90	217.0
135.00	331.0
136.70	223.0
137.10	244.0
140.00	183.0
140.90	1773.0
141.80	182.0
143.00	2755.0
144.00	224.0
144.90	1282.0
145.90	258.0
147.90	403.0
148.80	148.0
149.90	157.0
151.80	109.0
153.00	119.0
153.90	144.0
154.90	462.0
155.90	131.0
157.00	231.0
158.90	246.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

160.90	154.0
170.90	764.0
172.00	1651.0
173.00	1871.0
174.00	120248.0
175.00	9266.0
176.00	116968.0
177.00	7662.0
178.00	218.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

m/z	Abundance
36.00	1347.0
37.00	7259.0
38.00	6333.0
39.00	2534.0
40.00	299.0
43.10	128.0
44.00	1240.0
45.00	1501.0
46.00	222.0
47.10	1943.0
48.00	975.0
49.00	6079.0
50.00	28920.0
51.00	9344.0
52.00	433.0
53.00	177.0
54.10	114.0
54.90	379.0
56.00	2271.0
57.00	4279.0
58.00	105.0
60.00	1656.0
61.00	7504.0
62.00	8045.0
63.00	7027.0
64.00	1116.0
65.00	1288.0
65.90	222.0
67.00	500.0
68.00	16197.0
69.00	15966.0
70.00	1266.0
72.00	945.0
73.00	7651.0
74.00	25360.0
75.00	78176.0
76.10	7210.0
77.00	1054.0
77.90	535.0
79.00	6800.0
79.90	2142.0
80.90	7136.0
82.00	1393.0
82.90	181.0
86.00	388.0
87.00	6933.0
88.00	6422.0
90.90	626.0
92.00	4646.0
93.00	6583.0
94.00	18696.0
95.00	158080.0
96.10	9901.0
97.00	371.0
103.00	145.0
103.90	891.0
105.00	353.0
106.00	796.0
106.90	153.0
107.90	151.0
110.10	207.0
110.90	179.0
111.90	191.0
112.90	213.0
114.70	206.0
115.80	688.0
117.00	1465.0
117.90	724.0
119.00	1067.0
123.90	108.0
124.80	115.0
125.90	138.0
127.90	621.0
128.90	307.0
129.80	439.0
131.00	236.0
135.00	348.0
137.00	279.0
140.00	172.0
141.00	1457.0
141.80	176.0
143.00	2636.0
144.00	208.0
145.00	1260.0
145.90	285.0
146.70	110.0
147.90	497.0
148.80	115.0
149.80	170.0
153.00	113.0
153.80	108.0
154.90	414.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

157.00	251.0
159.00	256.0
160.90	168.0
171.00	675.0
172.00	1774.0
173.00	1810.0
174.00	119472.0
175.00	9336.0
176.00	117536.0
177.00	7605.0
178.00	185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232