
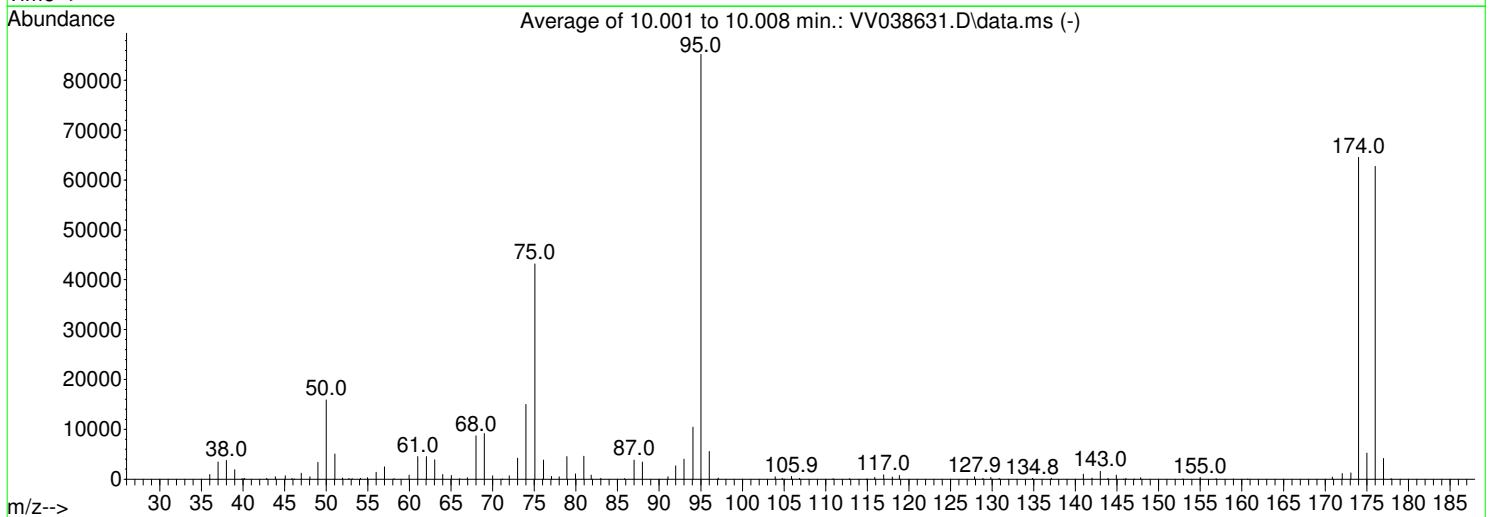


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020625\
 Data File : VV038631.D
 Acq On : 06 Feb 2025 14:01
 Operator : SY/MD
 Sample : BFB201
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB201

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Feb 17 10:31:04 2025

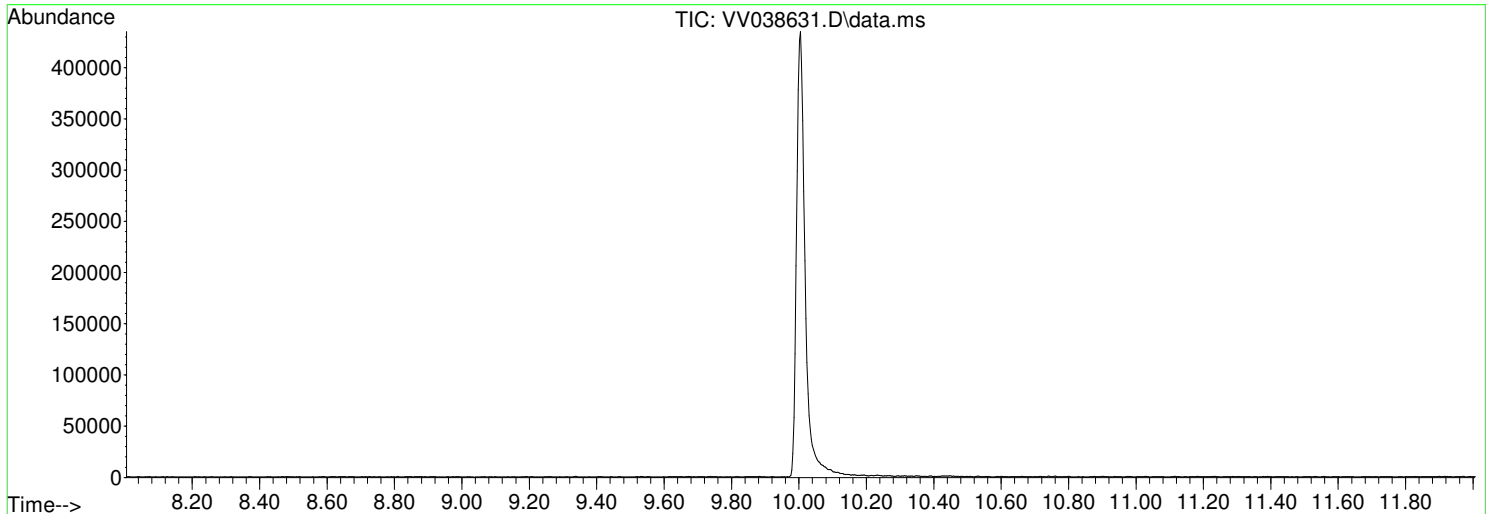

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2775

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	15887	PASS
75	95	30	80	50.6	43160	PASS
95	95	100	100	100.0	85227	PASS
96	95	5	9	6.5	5568	PASS
173	174	0.00	2	2.0	1283	PASS
174	95	50	120	75.7	64525	PASS
175	174	5	9	8.1	5217	PASS
176	174	95	105	97.3	62781	PASS
177	176	5	10	6.6	4127	PASS

Scan 2775 (9.963 min): VV038631.D\data.ms
BFB201

m/z	Abundance
39.90	138.0
43.90	392.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

m/z	Abundance
36.00	985.0
37.00	3643.0
38.00	3830.0
39.00	1736.0
39.80	283.0
40.20	287.0
42.80	122.0
43.90	820.0
45.10	684.0
46.20	181.0
47.00	1247.0
48.00	506.0
49.00	3554.0
50.00	16648.0
51.00	5254.0
51.90	288.0
52.70	149.0
53.10	151.0
54.10	104.0
54.90	303.0
56.00	1415.0
57.00	2602.0
58.10	142.0
59.90	814.0
61.00	4815.0
62.00	4618.0
63.10	4053.0
64.00	1005.0
65.10	724.0
66.00	116.0
66.90	264.0
68.00	8742.0
69.00	9060.0
70.00	642.0
71.20	112.0
72.00	722.0
73.00	4223.0
74.00	15551.0
75.00	43952.0
76.10	4092.0
77.10	605.0
78.00	538.0
78.90	4383.0
79.90	1012.0
81.00	4680.0
81.90	917.0
83.00	125.0
85.80	192.0
87.00	3763.0
88.00	3506.0
91.00	504.0
92.00	2499.0
93.00	4127.0
94.10	10600.0
95.00	87288.0
96.00	5624.0
97.10	168.0
103.90	512.0
104.70	105.0
105.90	488.0
106.80	127.0
112.80	103.0
114.90	117.0
115.90	398.0
117.00	913.0
118.00	453.0
118.80	749.0
127.90	440.0
128.90	176.0
129.80	351.0
130.90	161.0
134.80	174.0
137.10	195.0
140.90	985.0
142.00	209.0
143.00	1511.0
143.90	139.0
144.90	900.0
145.80	187.0
147.80	278.0
155.00	409.0
157.00	114.0
170.90	407.0
172.00	1143.0
173.10	1305.0
174.00	64112.0
175.00	5247.0
176.00	61152.0
177.00	4200.0
178.00	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

m/z	Abundance
36.00	980.0
37.00	3499.0
38.00	3915.0
39.00	1952.0
39.90	278.0
40.20	288.0
42.90	152.0
44.00	926.0
45.10	697.0
45.90	212.0
47.00	1296.0
48.00	507.0
49.00	3447.0
50.00	16349.0
51.10	5225.0
52.00	244.0
52.70	160.0
53.10	139.0
54.10	160.0
55.00	306.0
56.00	1452.0
57.00	2469.0
58.10	114.0
60.00	779.0
61.00	4647.0
62.00	4692.0
63.10	3988.0
64.00	924.0
65.10	731.0
66.10	113.0
66.90	316.0
68.00	8885.0
69.00	9508.0
70.00	688.0
72.00	735.0
73.00	4371.0
74.00	15366.0
75.00	44512.0
76.10	3877.0
77.10	614.0
78.00	493.0
78.90	4690.0
80.00	1112.0
81.00	4672.0
81.90	824.0
83.00	133.0
85.90	147.0
87.00	3980.0
88.00	3501.0
91.00	474.0
92.00	2777.0
93.00	4053.0
94.10	10757.0
95.00	87720.0
96.00	5698.0
97.10	234.0
104.00	508.0
104.80	131.0
105.90	562.0
106.90	142.0
110.90	116.0
112.80	119.0
115.90	394.0
117.00	879.0
118.00	402.0
118.80	754.0
127.90	501.0
128.90	186.0
129.80	411.0
130.80	181.0
134.90	172.0
137.10	202.0
140.90	1007.0
142.00	228.0
143.00	1690.0
143.90	143.0
144.90	814.0
146.00	213.0
147.80	300.0
155.00	355.0
156.90	125.0
170.80	465.0
172.00	1135.0
173.10	1325.0
174.00	66496.0
175.00	5453.0
176.00	64784.0
177.00	4225.0
177.90	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

m/z	Abundance
36.00	834.0
37.00	3272.0
38.00	3524.0
39.00	1962.0
40.00	318.0
42.90	145.0
44.00	973.0
45.10	639.0
45.90	192.0
47.00	1070.0
48.10	432.0
49.00	3039.0
50.00	14665.0
51.10	4637.0
52.00	205.0
52.80	174.0
54.10	185.0
55.00	286.0
56.00	1299.0
57.00	2293.0
58.20	114.0
60.00	795.0
61.00	4216.0
62.10	4318.0
63.00	3684.0
64.00	811.0
65.00	711.0
67.00	301.0
68.00	8524.0
69.00	8927.0
70.00	624.0
72.00	613.0
73.00	4076.0
74.00	13989.0
75.10	41016.0
76.10	3444.0
76.90	484.0
78.00	422.0
78.90	4518.0
80.00	1119.0
80.90	4332.0
81.80	682.0
83.00	160.0
87.00	3757.0
88.00	3386.0
91.10	385.0
92.00	2693.0
93.00	3886.0
94.00	9863.0
95.00	80672.0
96.00	5382.0
97.10	289.0
103.90	476.0
104.90	178.0
105.90	531.0
106.80	136.0
110.90	112.0
112.90	139.0
115.90	341.0
116.90	781.0
118.00	321.0
118.90	684.0
127.90	433.0
128.90	191.0
129.90	370.0
130.80	191.0
134.90	142.0
137.10	186.0
141.00	987.0
142.00	173.0
143.00	1586.0
143.90	157.0
144.90	651.0
146.10	257.0
147.10	124.0
147.90	277.0
152.90	105.0
155.00	260.0
156.80	132.0
159.00	105.0
160.70	116.0
170.80	444.0
172.10	1110.0
173.10	1218.0
174.00	62968.0
175.00	4951.0
176.00	62408.0
177.00	3956.0
178.00	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201