




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034046.D
Acq On : 08 Feb 2024 09:54
Operator : SY/MD
Sample : VV0208WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK210

Manual IntegrationsAPPROVED

Quant Time: Feb 09 00:40:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 09 00:39:09 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/09/2024
Supervised By :Mahesh Dadoda 02/09/2024

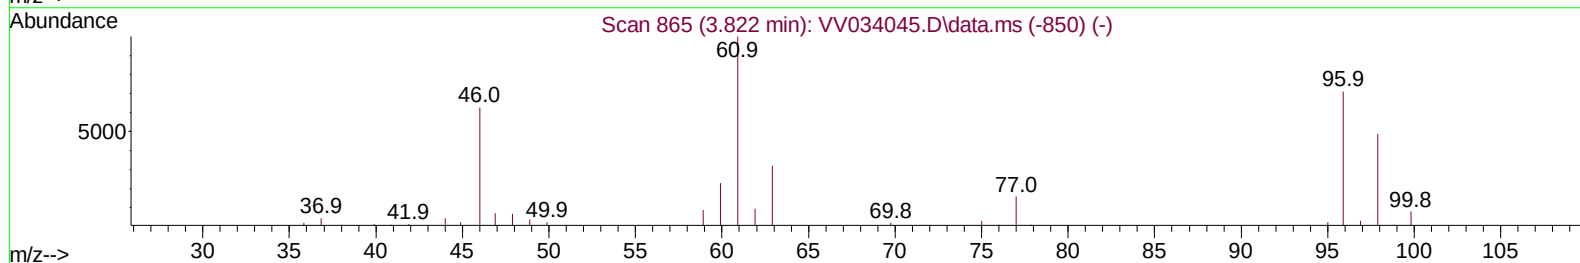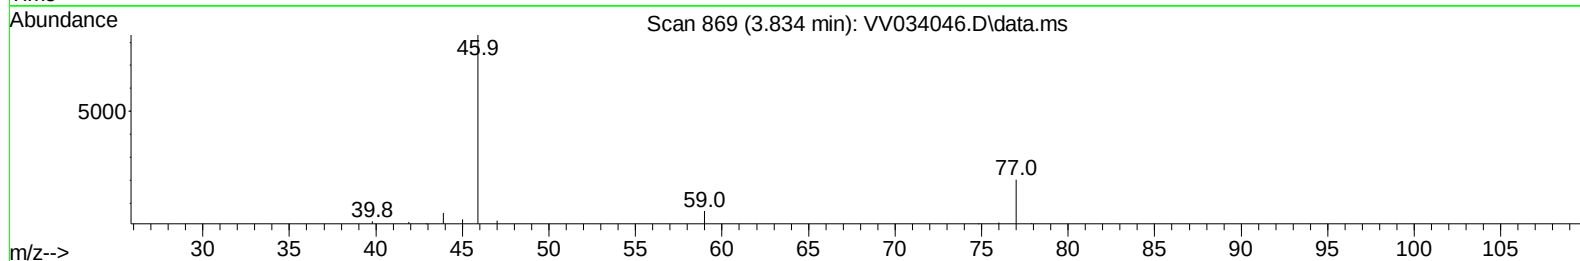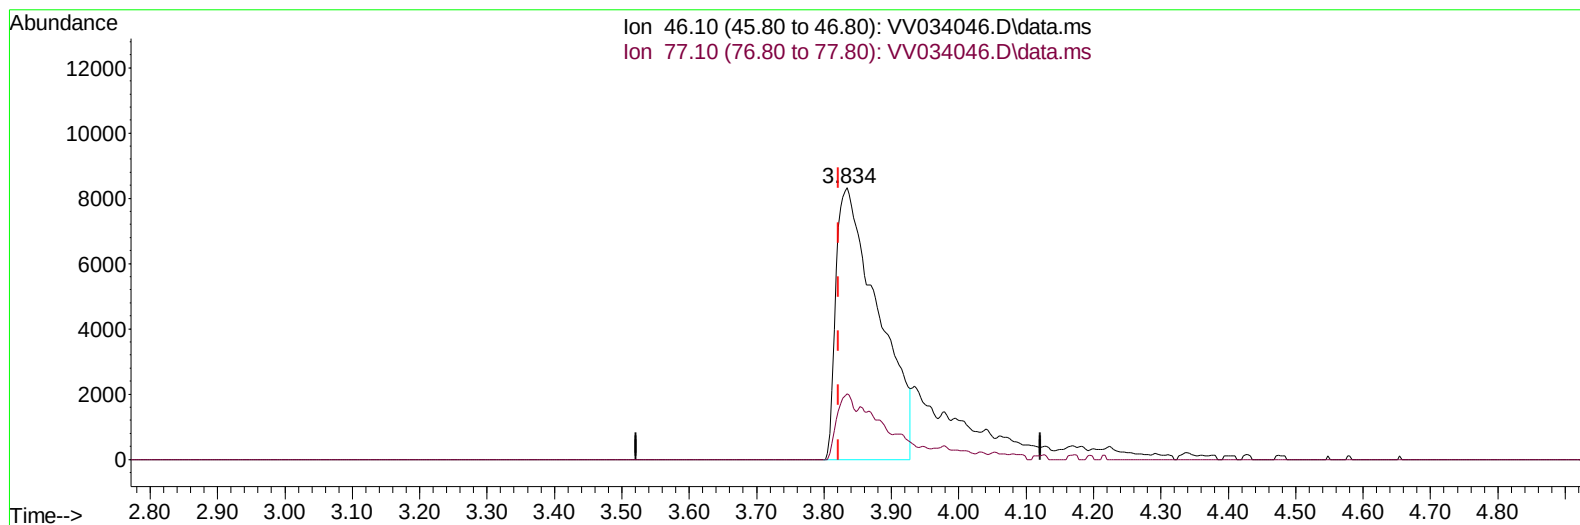

TIC: VV034046.D\data.ms

(20) 2-Butanone-d5 (S)

3.834min (+ 0.013) 32.68 ug/L

response 36138

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.80	9.95#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
 Data File : VV034046.D
 Acq On : 08 Feb 2024 09:54
 Operator : SY/MD
 Sample : VV0208WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK210

Manual IntegrationsAPPROVED

Quant Time: Feb 09 00:40:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 09 00:39:09 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/09/2024
 Supervised By :Mahesh Dadoda 02/09/2024

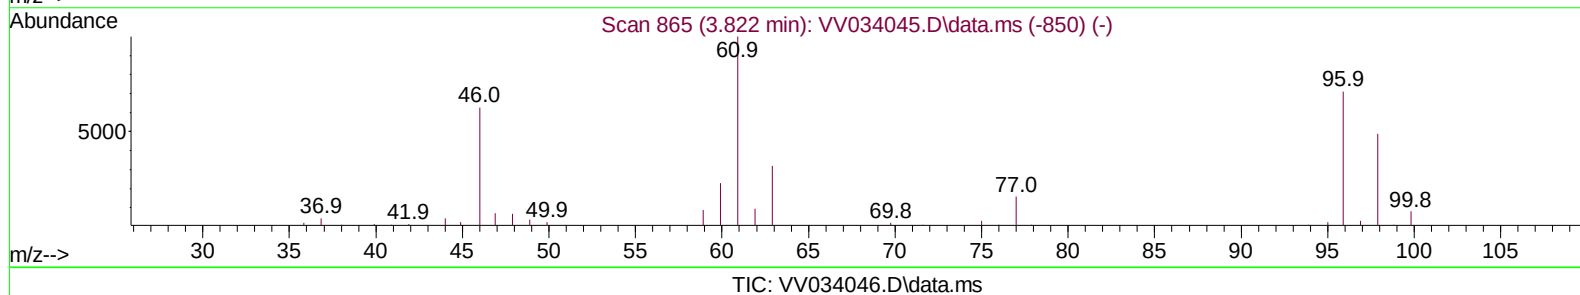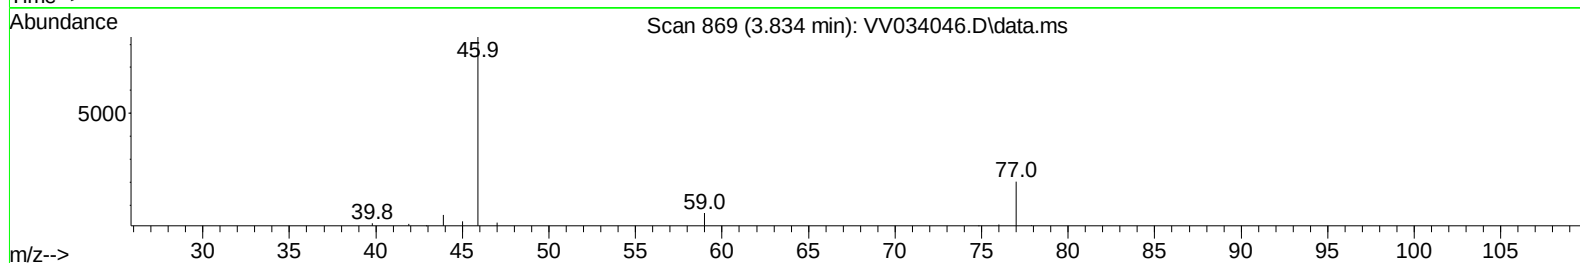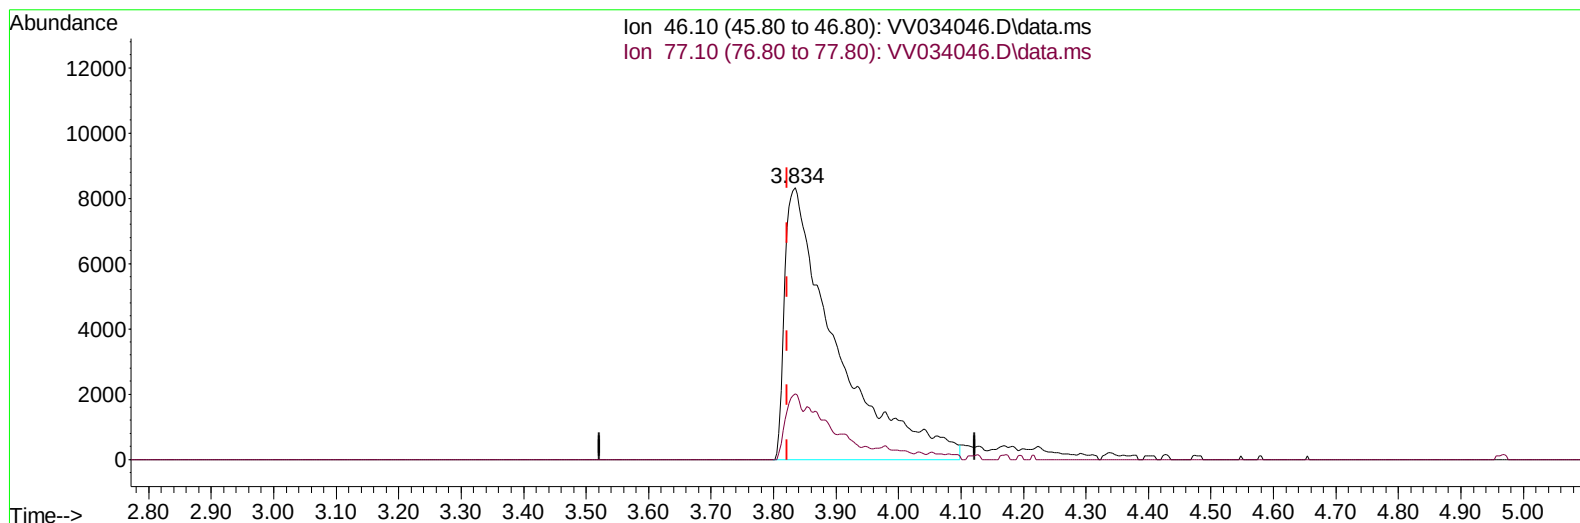

(20) 2-Butanone-d5 (S)

3.834min (+ 0.013) 42.88 ug/L m

response 47426

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.80	7.58#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
 Data File : VV034046.D
 Acq On : 08 Feb 2024 09:54
 Operator : SY/MD
 Sample : VV0208WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK210

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/09/2024
 Supervised By :Mahesh Dadoda 02/09/2024

Quant Time: Feb 09 00:40:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 09 00:39:09 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.535	114		85028	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117		77791	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152		38387	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		31507	4.785	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.600%	
7) Chloroethane-d5	1.532	69		25607	4.440	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.800%	
11) 1,1-Dichloroethene-d2	2.059	65		14854	4.677	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	93.600%	
20) 2-Butanone-d5	3.834	46		47426m	42.882	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.760%	
24) Chloroform-d	4.252	84		53453	4.467	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.400%	
26) 1,2-Dichloroethane-d4	4.947	65		26671	4.769	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.400%	
32) Benzene-d6	4.963	84		106833	4.577	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%	
36) 1,2-Dichloropropane-d6	5.992	67		28741	4.405	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.200%	
41) Toluene-d8	7.246	98		97030	4.524	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.400%	
43) trans-1,3-Dichloroprop...	7.558	79		11001	4.466	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.400%	
46) 2-Hexanone-d5	8.030	63		36926	41.990	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.980%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84		17108	4.325	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.600%	
66) 1,2-Dichlorobenzene-d4	11.561	152		32282	4.624	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.400%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034046.D
Acq On : 08 Feb 2024 09:54
Operator : SY/MD
Sample : VV0208WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK210

Manual IntegrationsAPPROVED

Quant Time: Feb 09 00:40:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 09 00:39:09 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/09/2024
Supervised By :Mahesh Dadoda 02/09/2024

