

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
 Data File : VV034049.D
 Acq On : 08 Feb 2024 11:24
 Operator : SY/MD
 Sample : P1400-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV034049.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rBV	34170	37527	13.99%	1.561%
2	1.536	146	154	164	rVB	34566	40788	15.20%	1.697%
3	2.063	307	318	332	rBV	78156	123023	45.85%	5.119%
4	2.519	451	460	466	rBV2	1737	2857	1.06%	0.119%
5	2.709	503	519	543	rVB3	14408	31764	11.84%	1.322%
6	3.117	635	646	664	rVB2	4627	9206	3.43%	0.383%
7	3.812	853	862	907	rBV2	22162	81130	30.24%	3.376%
8	4.256	983	1000	1028	rBV4	50897	150661	56.15%	6.269%
9	4.523	1069	1083	1093	rBV5	4657	10936	4.08%	0.455%
10	4.568	1093	1097	1106	rVB	3855	3579	1.33%	0.149%
11	4.960	1204	1219	1242	rBV2	108517	268305	100.00%	11.164%
12	5.539	1388	1399	1421	rBV	95737	199457	74.34%	8.299%
13	5.992	1529	1540	1567	rBV2	58644	123121	45.89%	5.123%
14	6.918	1818	1828	1854	rBV	27116	53584	19.97%	2.230%
15	7.246	1918	1930	1950	rBV	130380	231101	86.13%	9.616%
16	7.561	2020	2028	2051	rBV2	15359	29787	11.10%	1.239%
17	7.879	2118	2127	2139	rVB3	3262	5988	2.23%	0.249%
18	8.027	2165	2173	2213	rBV	116391	234379	87.36%	9.753%
19	8.786	2399	2409	2437	rBV	145884	246487	91.87%	10.256%
20	10.153	2822	2834	2853	rBV2	38877	62576	23.32%	2.604%
21	10.326	2879	2888	2900	rBV2	5430	9323	3.47%	0.388%
22	11.185	3145	3155	3184	rBV	156974	246803	91.99%	10.269%
23	11.561	3261	3272	3292	rBV	127174	200887	74.87%	8.359%




Sum of corrected areas: 2403269

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034049.D
Acq On : 08 Feb 2024 11:24
Operator : SY/MD
Sample : P1400-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

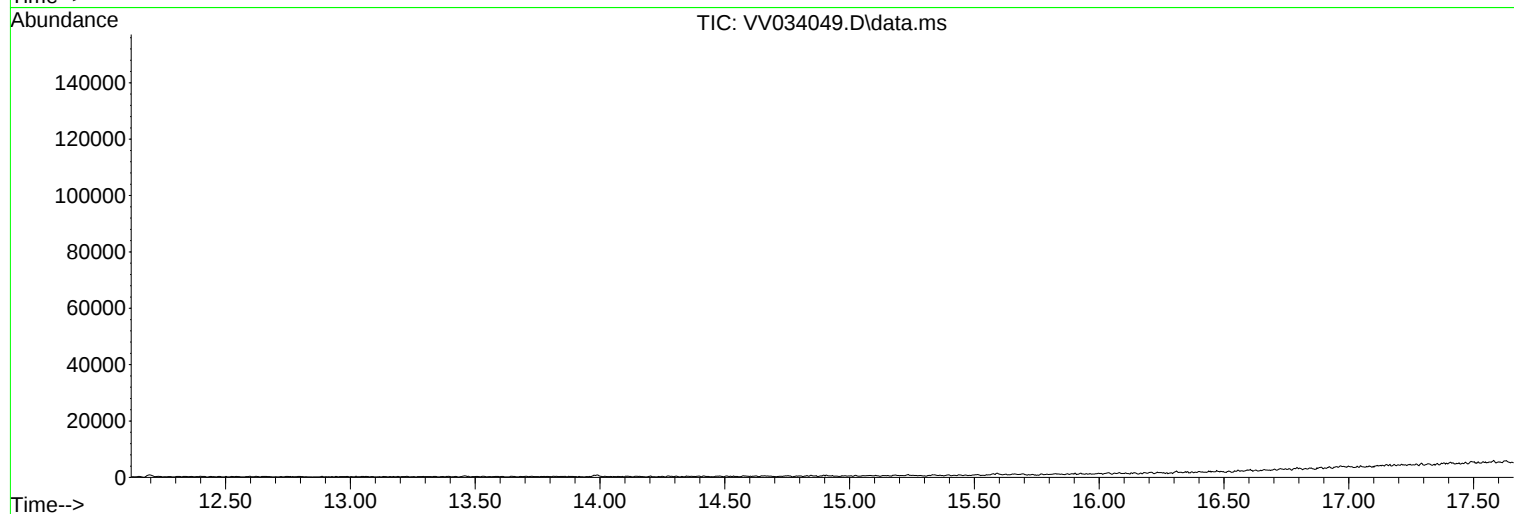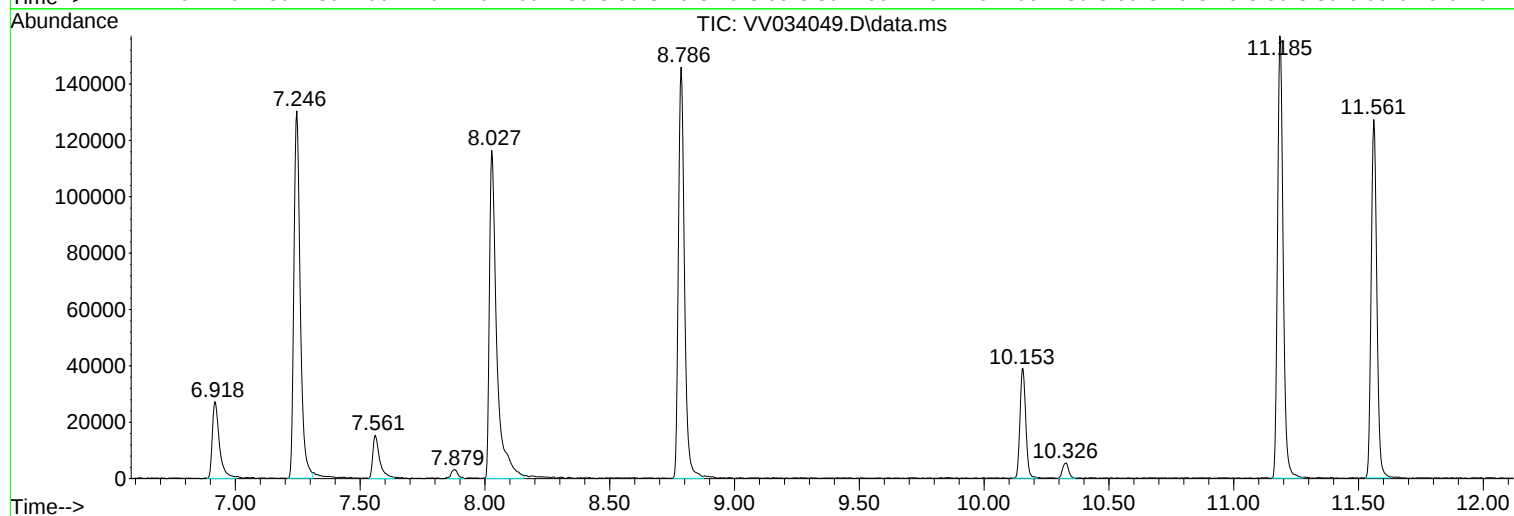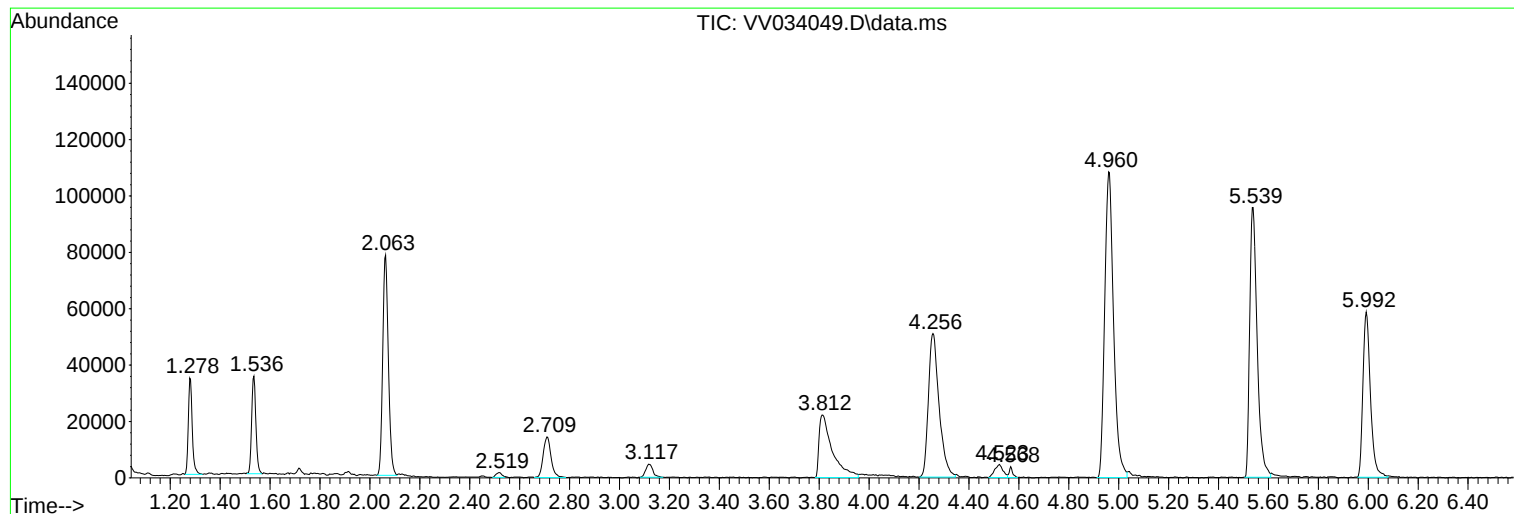

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034049.D
Acq On : 08 Feb 2024 11:24
Operator : SY/MD
Sample : P1400-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034049.D
Acq On : 08 Feb 2024 11:24
Operator : SY/MD
Sample : P1400-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
