

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
 Data File : VV034051.D
 Acq On : 08 Feb 2024 12:11
 Operator : SY/MD
 Sample : P1400-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034051.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.101	13	19	29	rVB	5819	6907	2.55%	0.295%
2	1.278	67	74	93	rVB	34882	37170	13.73%	1.588%
3	1.535	146	154	168	rVB	34333	42212	15.59%	1.803%
4	2.060	307	317	332	rBV	69603	101482	37.49%	4.335%
5	3.822	855	865	897	rBV2	19109	75517	27.90%	3.226%
6	4.252	983	999	1023	rBV2	46719	120822	44.63%	5.161%
7	4.960	1205	1219	1252	rBV2	107289	270716	100.00%	11.564%
8	5.535	1387	1398	1424	rBV	99222	204165	75.42%	8.721%
9	5.992	1528	1540	1561	rBV2	59556	126670	46.79%	5.411%
10	6.918	1819	1828	1850	rBV2	27387	54616	20.17%	2.333%
11	7.246	1919	1930	1961	rBV	132660	237296	87.65%	10.137%
12	7.561	2019	2028	2045	rBV2	15264	28395	10.49%	1.213%
13	7.882	2116	2128	2129	rBV3	2589	3756	1.39%	0.160%
14	7.908	2129	2136	2148	rVB2	8574	14938	5.52%	0.638%
15	8.027	2165	2173	2214	rBV	114671	242486	89.57%	10.358%
16	8.786	2399	2409	2431	rBV	149350	248007	91.61%	10.594%
17	10.156	2822	2835	2848	rBV2	41369	65371	24.15%	2.792%
18	10.326	2879	2888	2898	rVB3	4971	8134	3.00%	0.347%
19	11.188	3145	3156	3177	rBV	154164	249248	92.07%	10.647%
20	11.561	3262	3272	3296	rBV	128872	203068	75.01%	8.675%




Sum of corrected areas: 2340976

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034051.D
Acq On : 08 Feb 2024 12:11
Operator : SY/MD
Sample : P1400-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

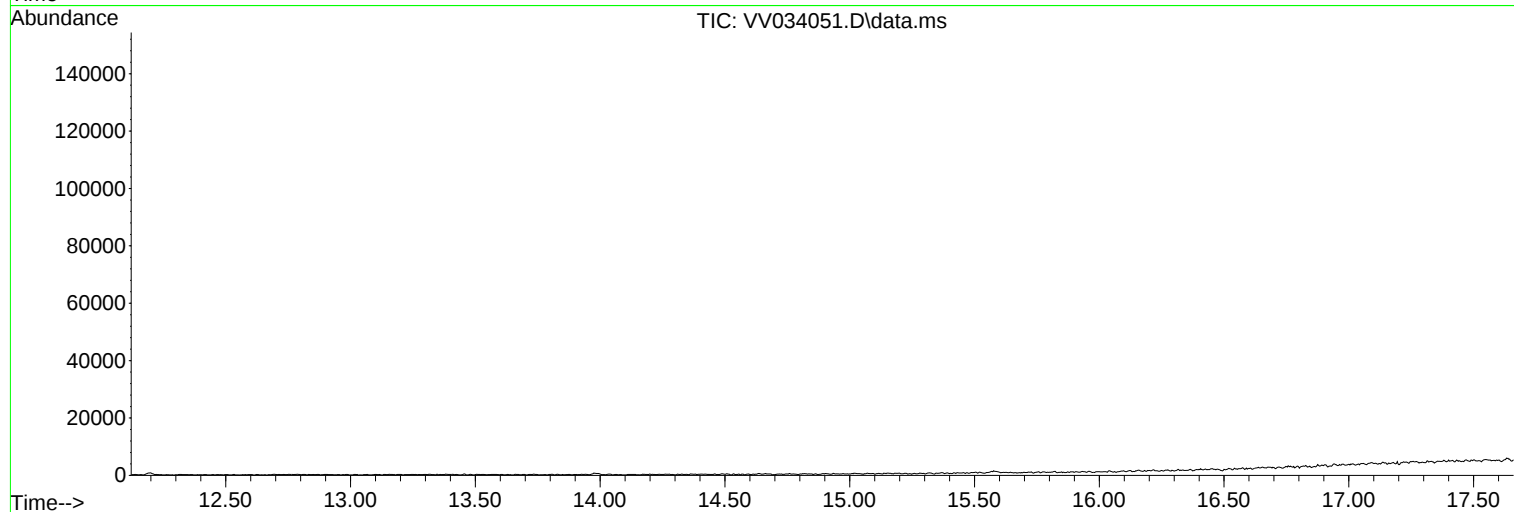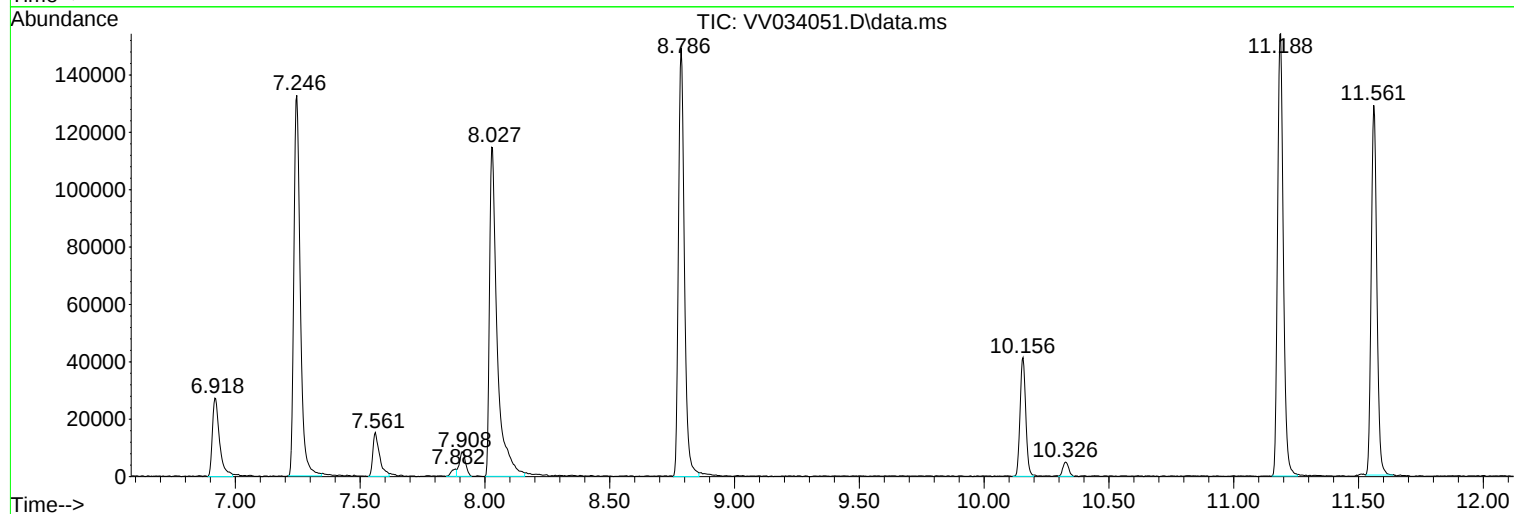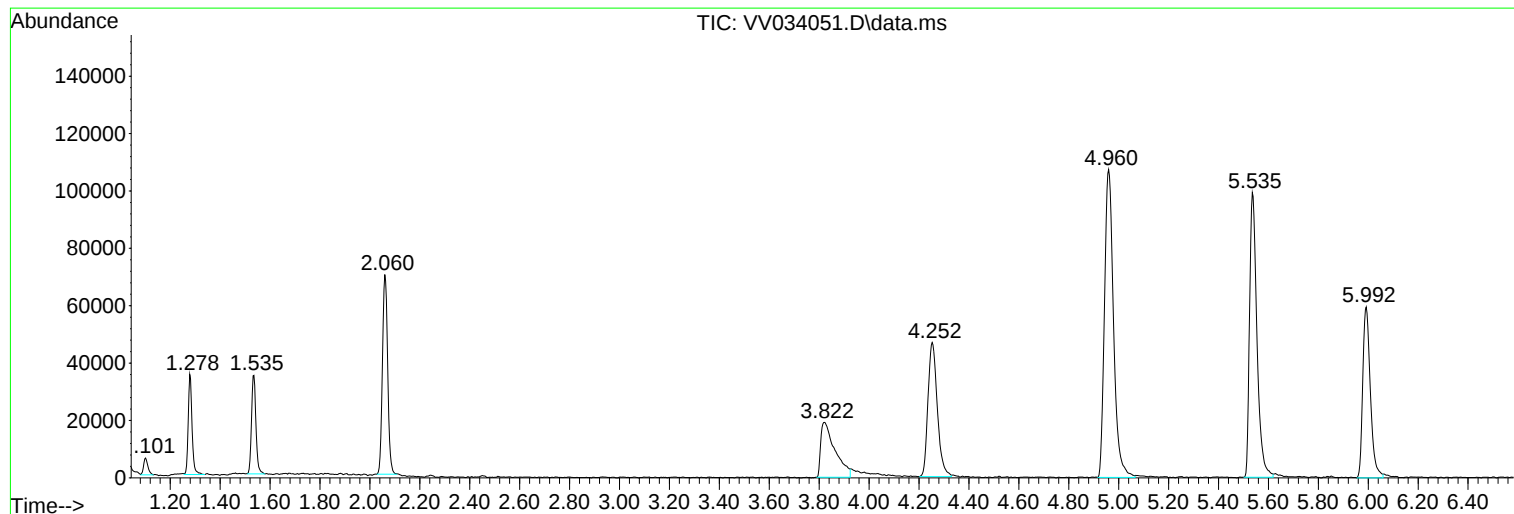

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034051.D
Acq On : 08 Feb 2024 12:11
Operator : SY/MD
Sample : P1400-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034051.D
Acq On : 08 Feb 2024 12:11
Operator : SY/MD
Sample : P1400-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc