

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
 Data File : VV034059.D
 Acq On : 08 Feb 2024 15:20
 Operator : SY/MD
 Sample : P1400-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	91	rVB	32325	35467	13.37%	1.551%
2	1.532	146	153	169	rVB	33288	40187	15.15%	1.758%
3	2.060	306	317	332	rBV	66636	97167	36.63%	4.250%
4	2.516	449	459	468	rBV6	1962	3910	1.47%	0.171%
5	3.809	853	861	901	rBV2	23628	83084	31.32%	3.634%
6	4.021	914	927	932	rBV6	1383	2890	1.09%	0.126%
7	4.252	984	999	1026	rBV	45982	118657	44.73%	5.190%
8	4.960	1203	1219	1249	rBV2	104623	265287	100.00%	11.604%
9	5.535	1387	1398	1425	rBV	95690	196178	73.95%	8.581%
10	5.992	1528	1540	1559	rBV2	57444	120759	45.52%	5.282%
11	6.918	1818	1828	1854	rBV	27460	53221	20.06%	2.328%
12	7.246	1919	1930	1960	rBV	126429	226412	85.35%	9.904%
13	7.561	2020	2028	2049	rBV2	14900	27679	10.43%	1.211%
14	7.876	2118	2126	2136	rVB2	3248	5241	1.98%	0.229%
15	8.027	2164	2173	2208	rBV	123326	248126	93.53%	10.853%
16	8.786	2399	2409	2440	rBV	143198	241013	90.85%	10.542%
17	10.156	2825	2835	2850	rBV	41159	65141	24.55%	2.849%
18	10.329	2877	2889	2901	rBV3	7305	11682	4.40%	0.511%
19	11.188	3145	3156	3178	rBV	152904	242878	91.55%	10.624%
20	11.561	3260	3272	3300	rVB	126516	201191	75.84%	8.800%




Sum of corrected areas: 2286170

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034059.D
Acq On : 08 Feb 2024 15:20
Operator : SY/MD
Sample : P1400-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

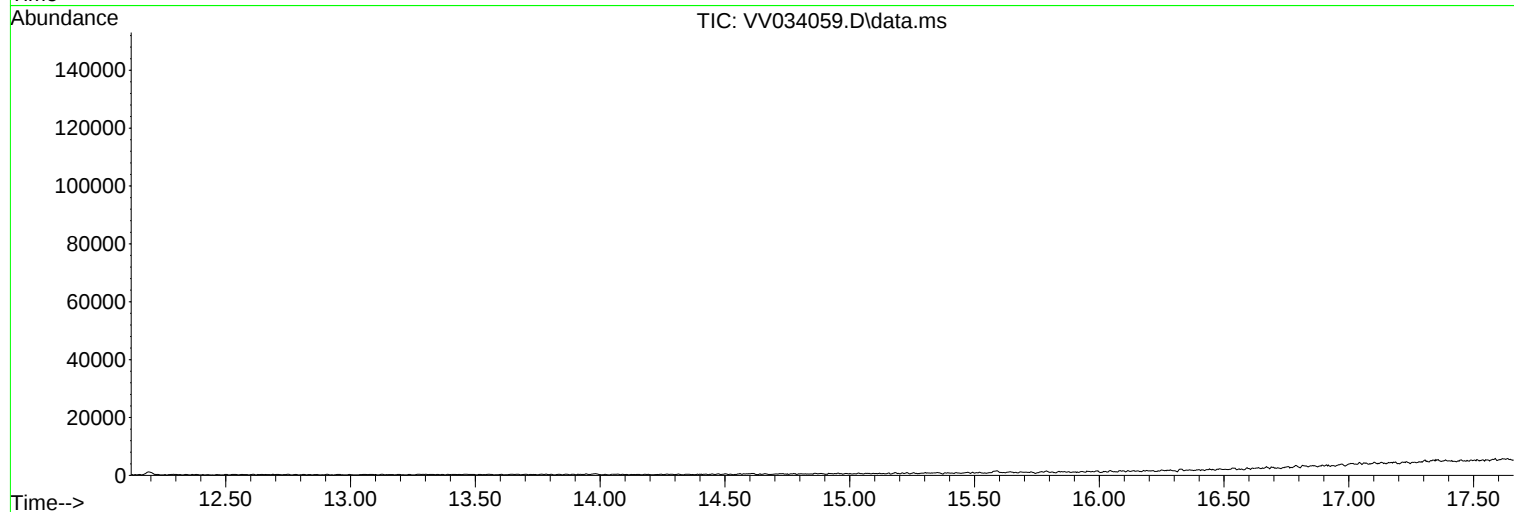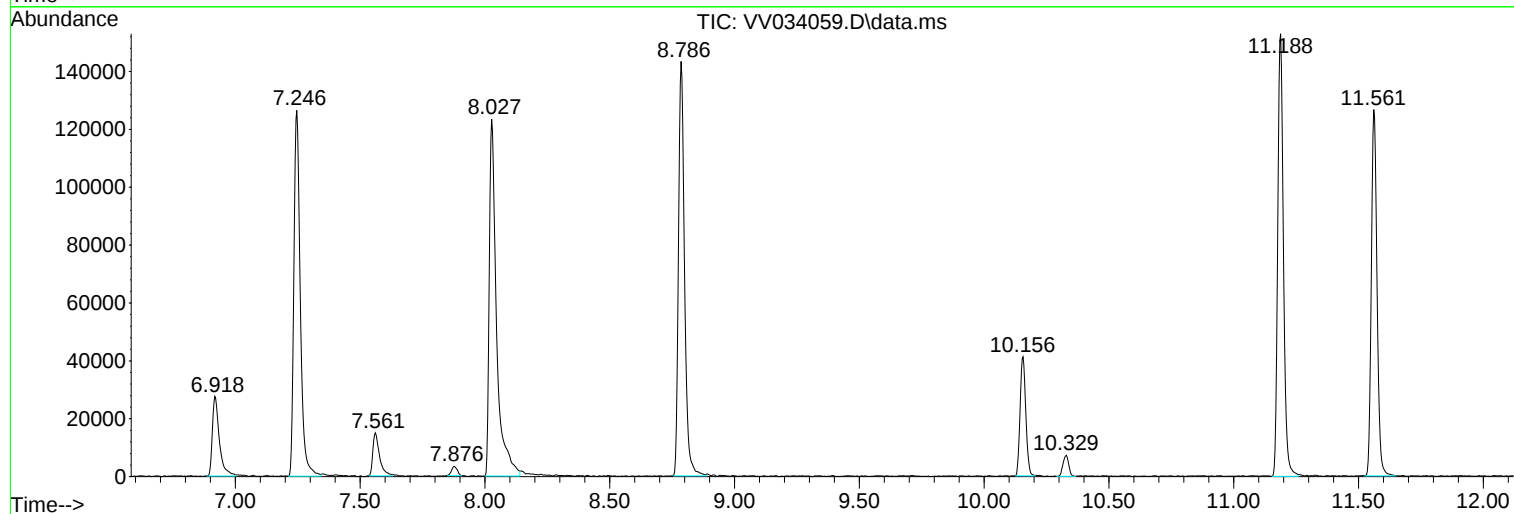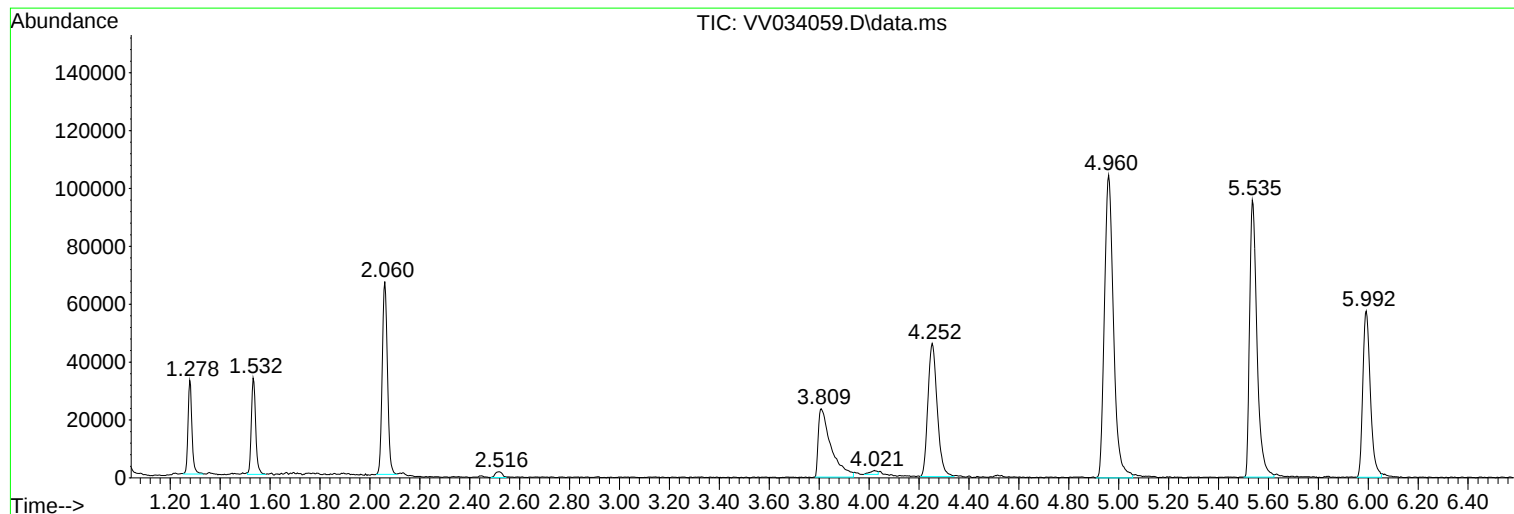

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034059.D
Acq On : 08 Feb 2024 15:20
Operator : SY/MD
Sample : P1400-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034059.D
Acq On : 08 Feb 2024 15:20
Operator : SY/MD
Sample : P1400-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc