

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
 Data File : VV034064.D
 Acq On : 08 Feb 2024 17:20
 Operator : SY/MD
 Sample : P1400-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV034064.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rBV	33667	35157	13.53%	1.442%
2	1.532	146	153	165	rVB	32958	38140	14.68%	1.564%
3	2.060	306	317	330	rBV	66298	96192	37.02%	3.945%
4	2.137	330	341	383	rVB2	24303	76590	29.47%	3.141%
5	2.516	452	459	470	rVB3	1716	3037	1.17%	0.125%
6	3.815	854	863	905	rBV	22551	85862	33.04%	3.521%
7	4.252	979	999	1023	rBV2	44061	119551	46.01%	4.903%
8	4.960	1201	1219	1244	rBV3	103153	259850	100.00%	10.656%
9	5.535	1385	1398	1421	rBV	91397	189102	72.77%	7.755%
10	5.992	1528	1540	1569	rBV2	58061	122062	46.97%	5.006%
11	6.918	1819	1828	1853	rBV2	26523	52416	20.17%	2.149%
12	7.246	1919	1930	1950	rBV	121270	218803	84.20%	8.973%
13	7.561	2017	2028	2047	rBV2	14754	27791	10.70%	1.140%
14	7.876	2115	2126	2137	rBV2	3042	5353	2.06%	0.220%
15	8.027	2165	2173	2206	rBV	121031	246019	94.68%	10.089%
16	8.252	2232	2243	2258	rBV3	10745	20861	8.03%	0.855%
17	8.786	2398	2409	2434	rBV	139053	233531	89.87%	9.577%
18	8.956	2453	2462	2476	rVB2	4368	7268	2.80%	0.298%
19	9.079	2487	2500	2522	rBV3	21567	38091	14.66%	1.562%
20	9.484	2618	2626	2637	rBV	8588	13390	5.15%	0.549%
21	10.156	2825	2835	2851	rBV	40987	64573	24.85%	2.648%
22	10.326	2871	2888	2900	rBV3	6910	13180	5.07%	0.540%
23	10.390	2900	2908	2915	rBV	7478	11790	4.54%	0.483%
24	10.480	2928	2936	2947	rVB2	2877	4002	1.54%	0.164%
25	10.683	2990	2999	3010	rVB3	2539	3575	1.38%	0.147%
26	10.857	3045	3053	3073	rVB2	10656	16251	6.25%	0.666%
27	11.188	3145	3156	3179	rBV	149663	237086	91.24%	9.722%
28	11.561	3262	3272	3294	rVB	123930	199022	76.59%	8.162%




Sum of corrected areas: 2438545

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034064.D
Acq On : 08 Feb 2024 17:20
Operator : SY/MD
Sample : P1400-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

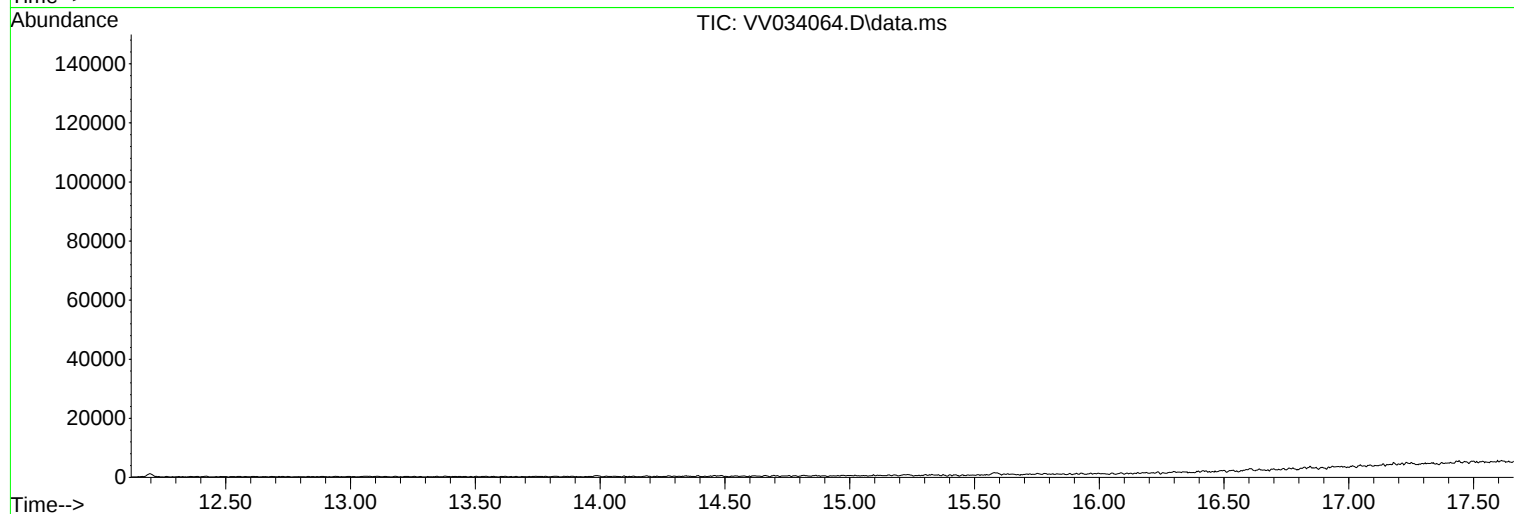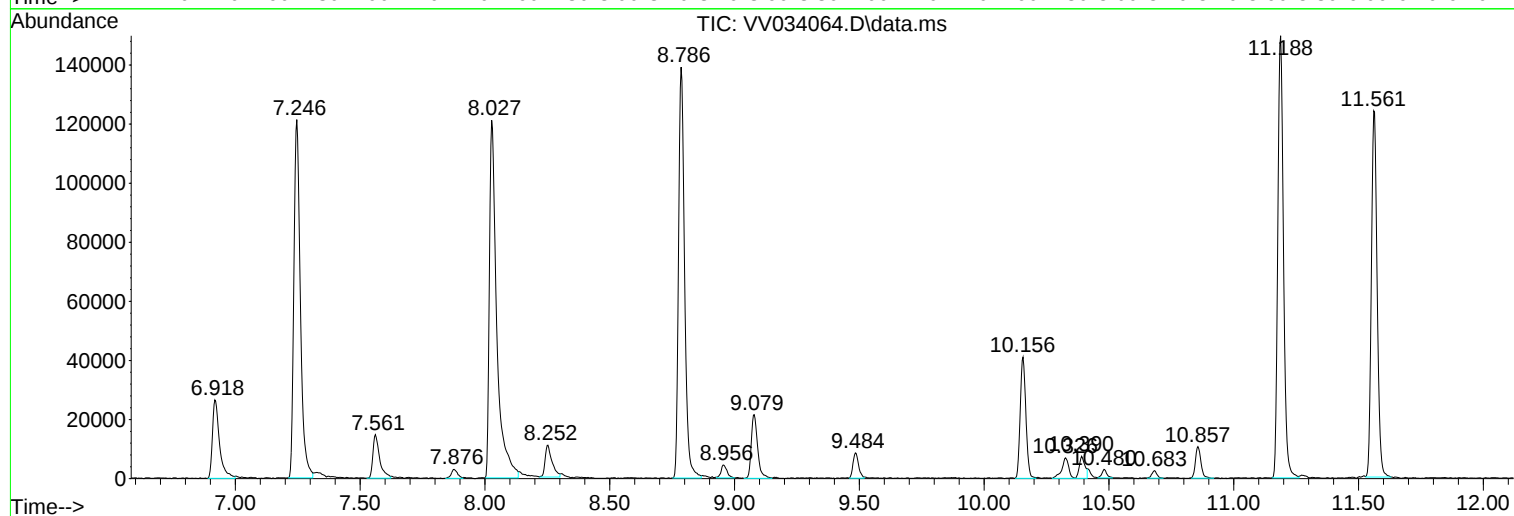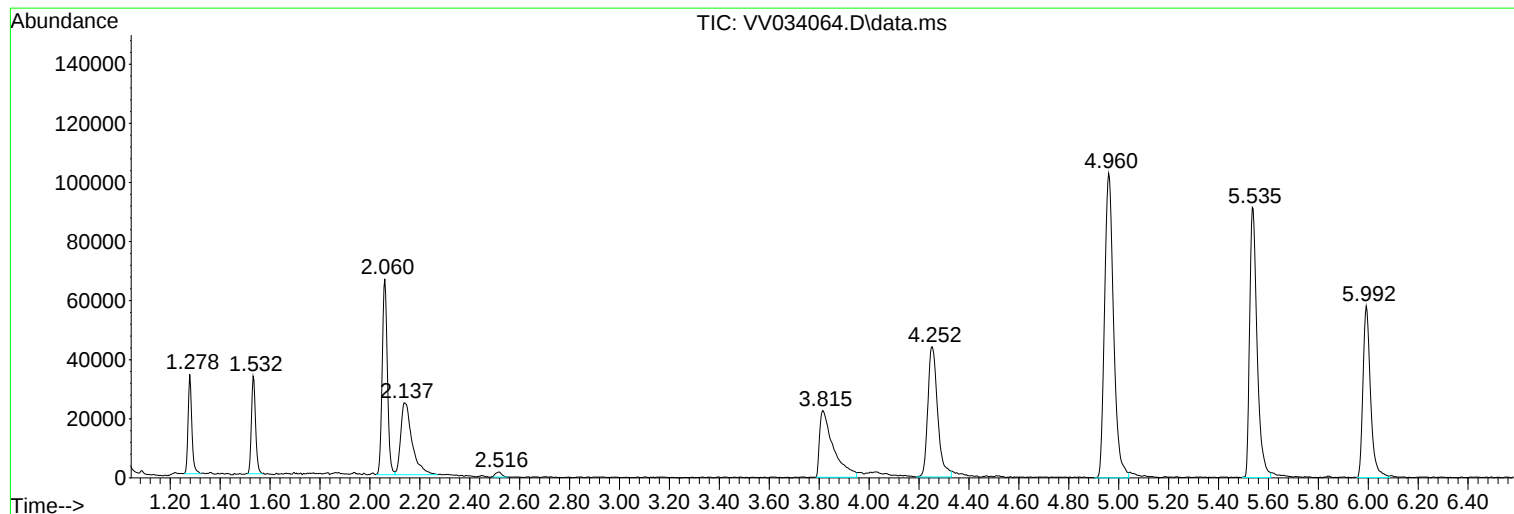

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034064.D
Acq On : 08 Feb 2024 17:20
Operator : SY/MD
Sample : P1400-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034064.D
Acq On : 08 Feb 2024 17:20
Operator : SY/MD
Sample : P1400-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc