

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
 Data File : VV034069.D
 Acq On : 08 Feb 2024 19:21
 Operator : SY/MD
 Sample : P1400-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV034069.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	38167	41088	13.07%	1.524%
2	1.532	146	153	169	rVB	38262	45137	14.35%	1.674%
3	2.060	306	317	333	rBV	74591	110733	35.22%	4.106%
4	2.127	333	338	346	rVV6	1842	3206	1.02%	0.119%
5	2.185	348	356	365	rVB	3643	5873	1.87%	0.218%
6	3.815	854	863	901	rBV2	26481	102450	32.58%	3.799%
7	4.252	983	999	1024	rBV	54850	138487	44.04%	5.135%
8	4.960	1205	1219	1254	rBV2	123215	314437	100.00%	11.659%
9	5.535	1388	1398	1426	rBV	107821	229302	72.92%	8.502%
10	5.992	1528	1540	1568	rBV	68774	145521	46.28%	5.396%
11	6.918	1819	1828	1851	rBV2	29872	61543	19.57%	2.282%
12	7.246	1917	1930	1951	rBV	147755	265908	84.57%	9.860%
13	7.561	2019	2028	2053	rBV	16720	32522	10.34%	1.206%
14	7.879	2115	2127	2139	rBV	3847	6938	2.21%	0.257%
15	8.027	2164	2173	2214	rBV	148618	299615	95.29%	11.109%
16	8.786	2397	2409	2436	rBV	166520	281891	89.65%	10.452%
17	10.156	2824	2835	2852	rBV	48479	76973	24.48%	2.854%
18	10.326	2879	2888	2901	rVB	9084	13666	4.35%	0.507%
19	11.188	3145	3156	3179	rBV	175588	281632	89.57%	10.443%
20	11.513	3247	3257	3262	rBV4	2014	3520	1.12%	0.131%
21	11.564	3262	3273	3296	rVB	145802	236503	75.21%	8.769%




Sum of corrected areas: 2696945

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034069.D
Acq On : 08 Feb 2024 19:21
Operator : SY/MD
Sample : P1400-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

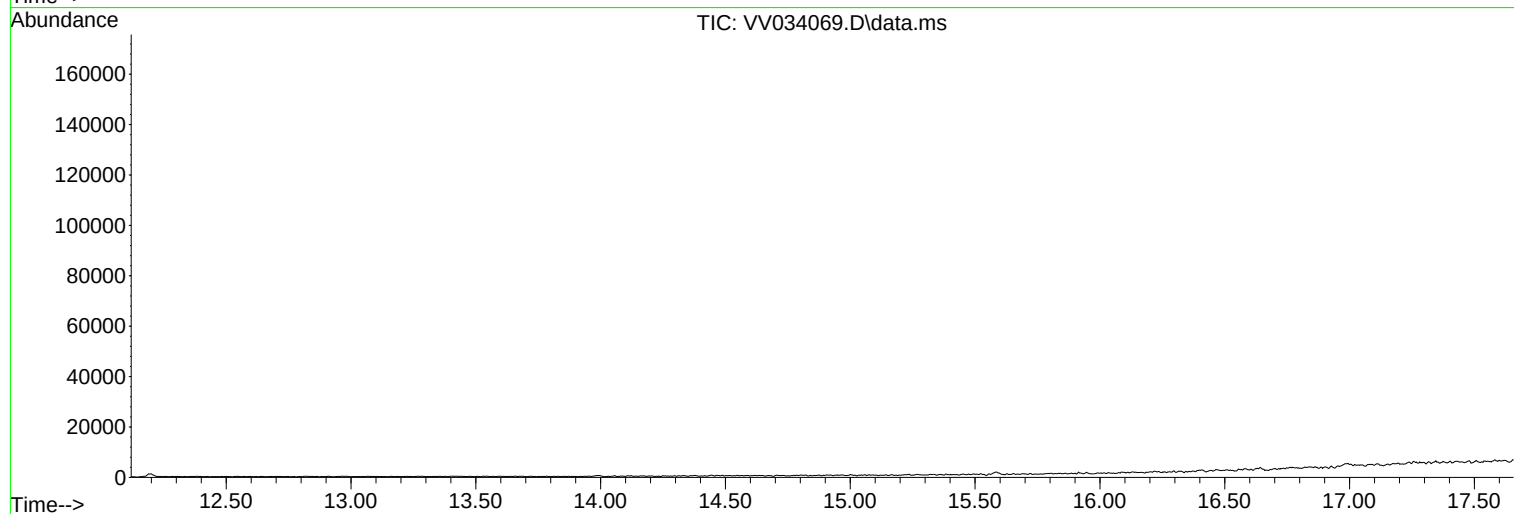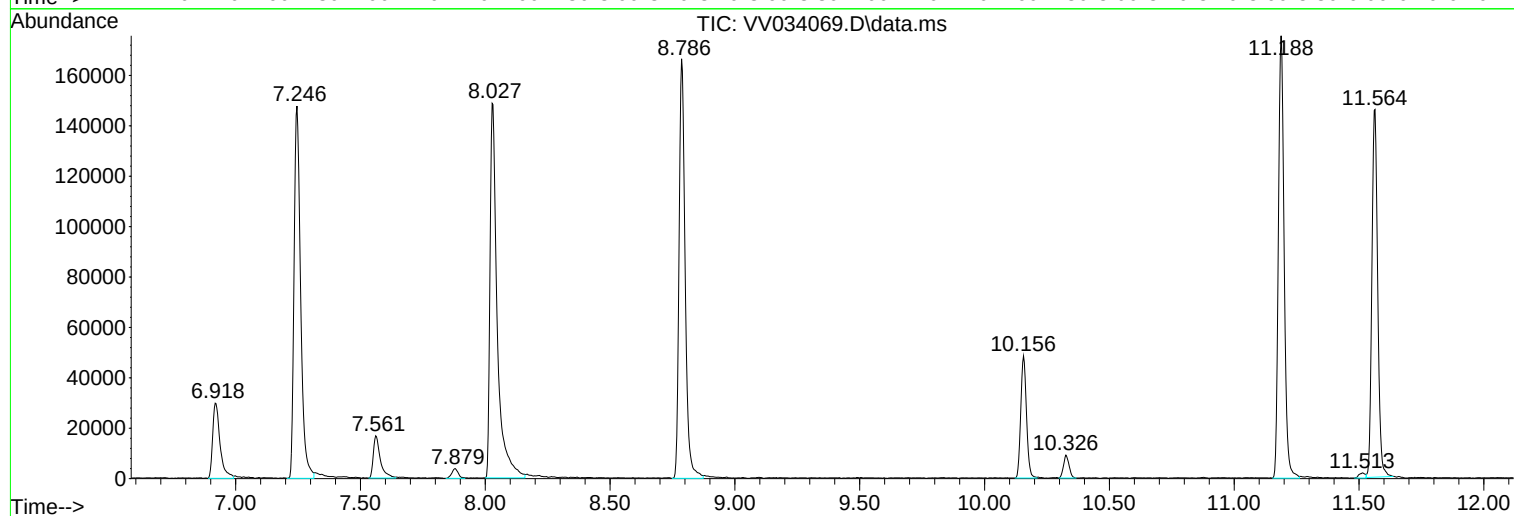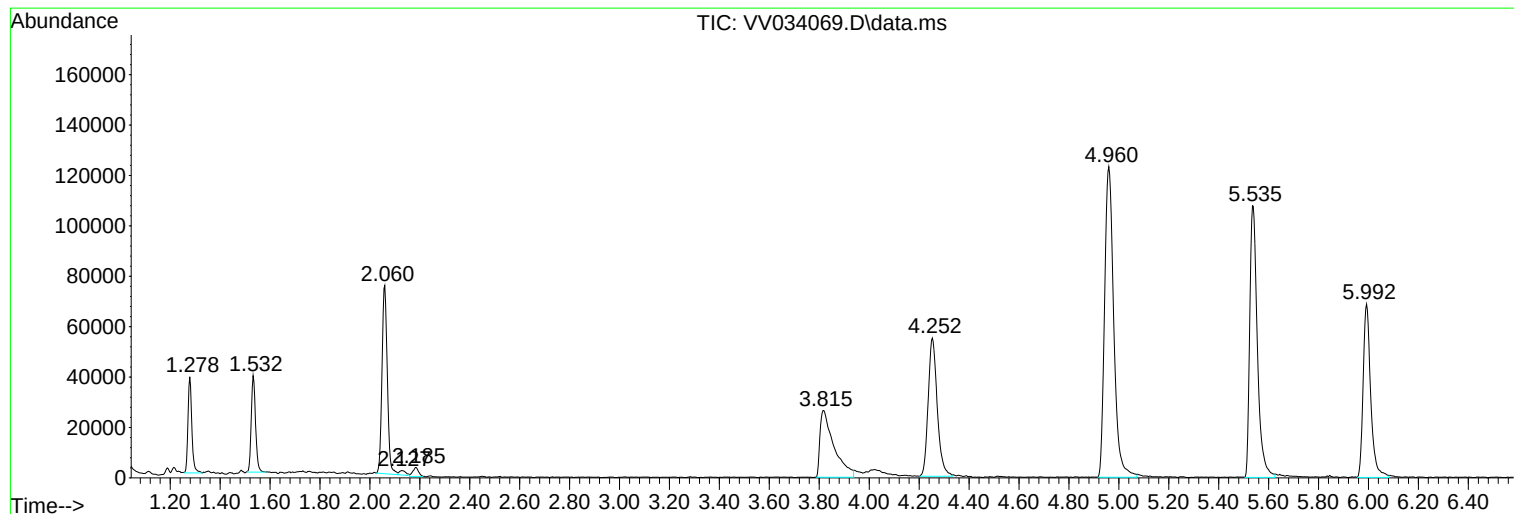

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034069.D
Acq On : 08 Feb 2024 19:21
Operator : SY/MD
Sample : P1400-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034069.D
Acq On : 08 Feb 2024 19:21
Operator : SY/MD
Sample : P1400-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
