

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
 Data File : VV034075.D
 Acq On : 08 Feb 2024 22:08
 Operator : SY/MD
 Sample : P1401-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV034075.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	87	rBV	35250	38110	14.02%	1.550%
2	1.532	145	153	166	rBV	34833	41187	15.15%	1.675%
3	2.060	308	317	334	rBV	69900	101457	37.32%	4.127%
4	2.709	506	519	538	rBV	21695	44455	16.35%	1.808%
5	3.121	637	647	656	rBV2	1783	3011	1.11%	0.122%
6	3.802	850	859	898	rBV3	30610	99292	36.52%	4.039%
7	4.252	985	999	1027	rBV2	48927	135054	49.68%	5.494%
8	4.960	1205	1219	1252	rBV3	107135	271868	100.00%	11.060%
9	5.539	1388	1399	1423	rBV	96166	197786	72.75%	8.046%
10	5.847	1487	1495	1510	rBV5	3114	6566	2.42%	0.267%
11	5.992	1526	1540	1574	rBV	61078	128873	47.40%	5.243%
12	6.921	1819	1829	1857	rBV2	25996	54434	20.02%	2.214%
13	7.246	1919	1930	1954	rBV	127280	229775	84.52%	9.347%
14	7.561	2020	2028	2046	rBV2	14463	28166	10.36%	1.146%
15	7.908	2127	2136	2150	rVB3	20391	35760	13.15%	1.455%
16	8.027	2164	2173	2212	rBV	133433	266586	98.06%	10.845%
17	8.786	2399	2409	2432	rBV	143853	243006	89.38%	9.886%
18	10.156	2825	2835	2849	rBV	43537	68825	25.32%	2.800%
19	10.329	2877	2889	2898	rVB	3048	4774	1.76%	0.194%
20	11.188	3145	3156	3179	rBV	156657	250035	91.97%	10.171%
21	11.564	3262	3273	3296	rVB	131206	209177	76.94%	8.509%




Sum of corrected areas: 2458197

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034075.D
Acq On : 08 Feb 2024 22:08
Operator : SY/MD
Sample : P1401-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

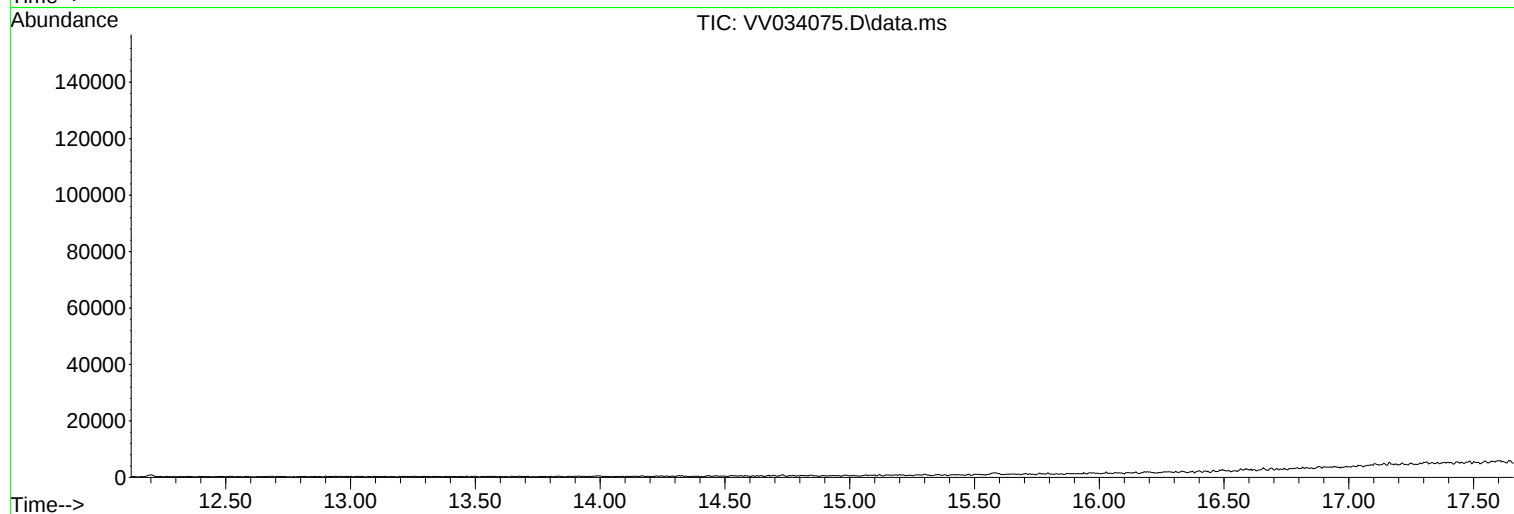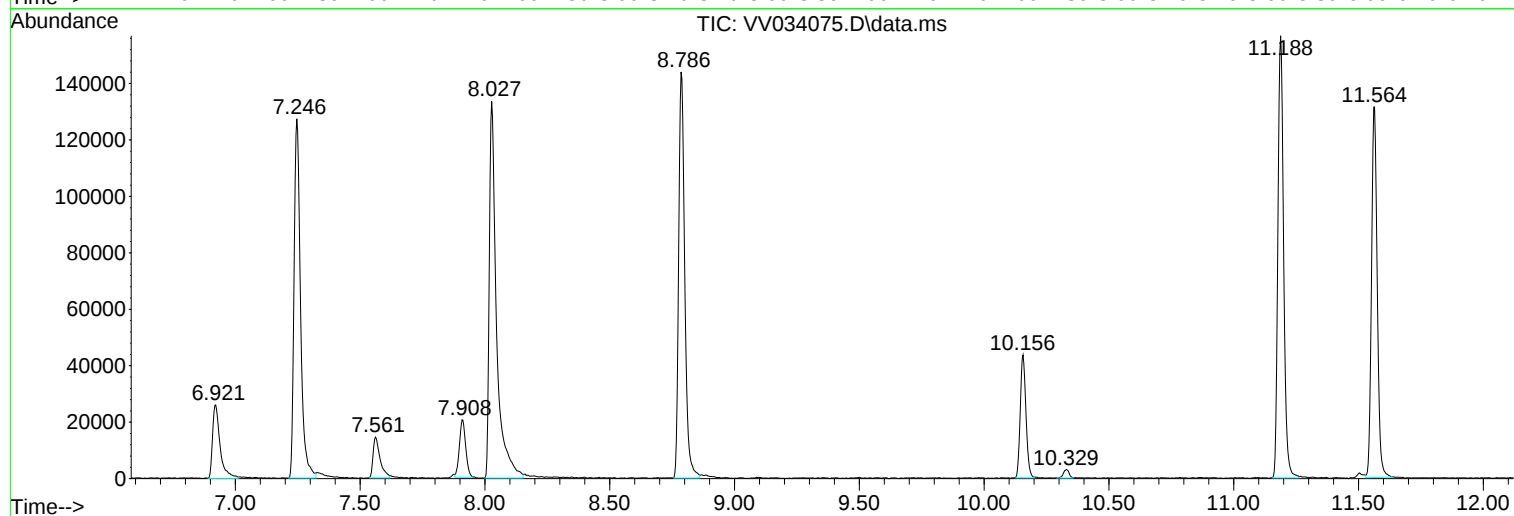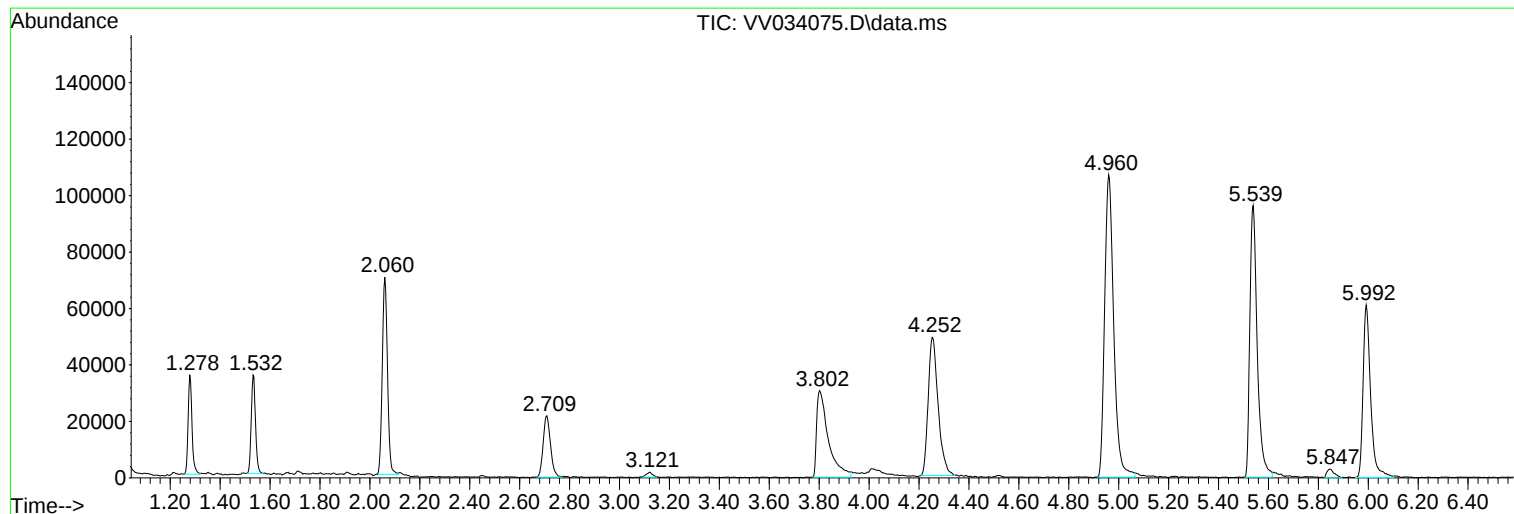

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034075.D
Acq On : 08 Feb 2024 22:08
Operator : SY/MD
Sample : P1401-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034075.D
Acq On : 08 Feb 2024 22:08
Operator : SY/MD
Sample : P1401-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc