

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
 Data File : VV034076.D
 Acq On : 08 Feb 2024 22:32
 Operator : SY/MD
 Sample : P1401-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034076.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rBV	34953	36970	13.58%	1.536%
2	1.532	145	153	168	rBV	35230	42077	15.45%	1.748%
3	2.056	306	316	333	rBV	71782	104121	38.24%	4.325%
4	3.818	855	864	903	rBV	21776	88220	32.40%	3.665%
5	4.252	984	999	1021	rBV3	47090	122091	44.84%	5.072%
6	4.960	1205	1219	1245	rBV2	108791	271820	99.83%	11.291%
7	5.539	1387	1399	1418	rBV	96057	198689	72.97%	8.253%
8	5.992	1528	1540	1570	rBV2	59972	129375	47.52%	5.374%
9	6.921	1820	1829	1853	rBV	25139	52727	19.37%	2.190%
10	7.246	1920	1930	1951	rBV	127908	231405	84.99%	9.612%
11	7.564	2017	2029	2047	rBV2	14064	28221	10.37%	1.172%
12	7.876	2116	2126	2140	rBV	8686	15030	5.52%	0.624%
13	8.030	2164	2174	2222	rBV	128288	272270	100.00%	11.310%
14	8.786	2398	2409	2441	rBV	148889	252834	92.86%	10.502%
15	10.156	2825	2835	2851	rBV	44280	70770	25.99%	2.940%
16	10.326	2877	2888	2899	rBV2	16014	25079	9.21%	1.042%
17	11.188	3146	3156	3181	rBV	160813	253666	93.17%	10.537%
18	11.561	3262	3272	3288	rBV	131523	208666	76.64%	8.668%
19	12.201	3460	3471	3480	rVB2	1920	3359	1.23%	0.140%




Sum of corrected areas: 2407390

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034076.D
Acq On : 08 Feb 2024 22:32
Operator : SY/MD
Sample : P1401-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

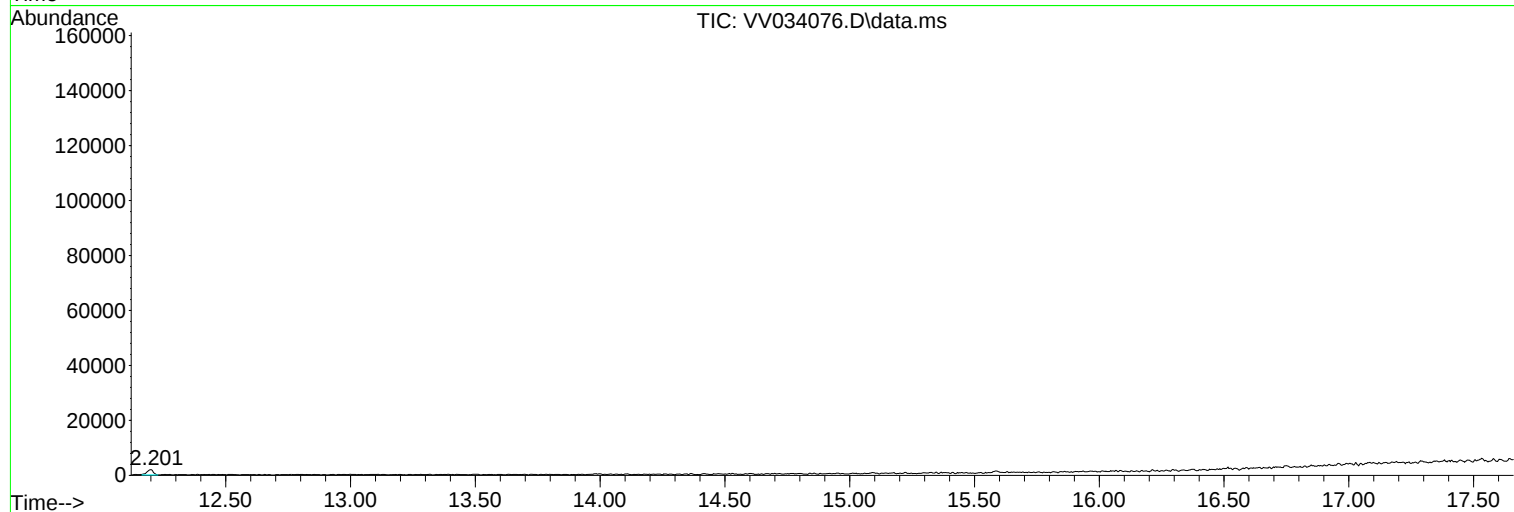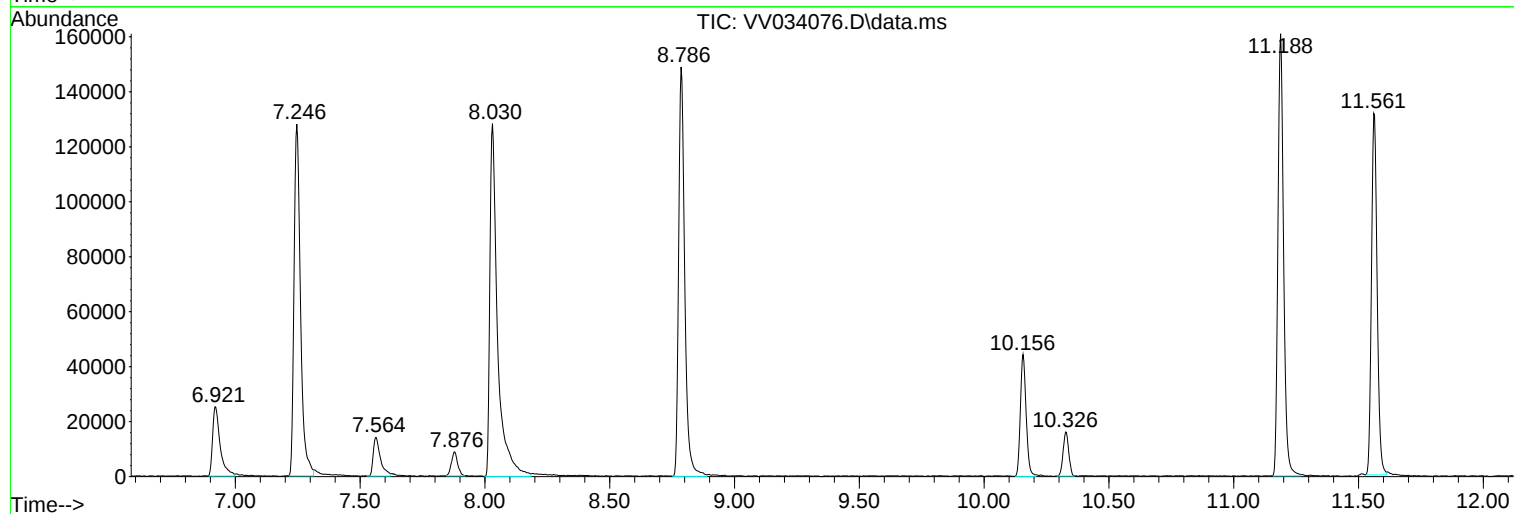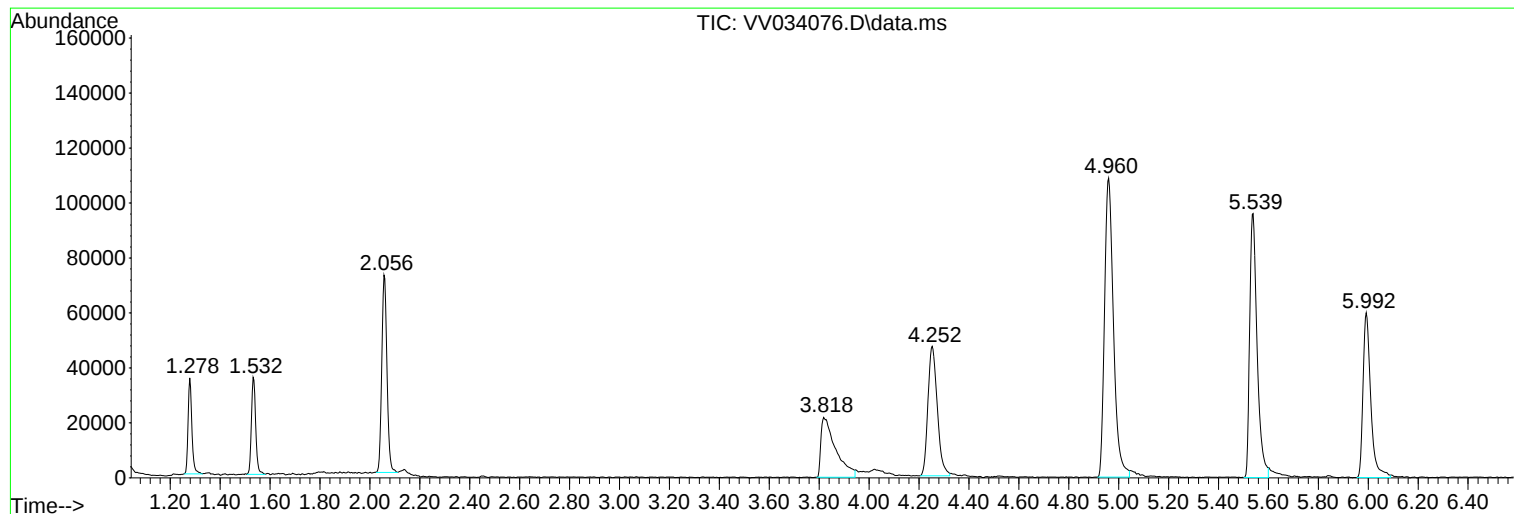

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034076.D
Acq On : 08 Feb 2024 22:32
Operator : SY/MD
Sample : P1401-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034076.D
Acq On : 08 Feb 2024 22:32
Operator : SY/MD
Sample : P1401-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc