

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
 Data File : VV034077.D
 Acq On : 08 Feb 2024 22:56
 Operator : SY/MD
 Sample : P1401-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV034077.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.102	13	19	35	rVB	6127	8192	3.03%	0.339%
2	1.278	67	74	91	rBV	33343	36549	13.54%	1.510%
3	1.532	143	153	164	rBV	34327	41049	15.21%	1.696%
4	2.060	302	317	331	rBV	68627	102089	37.82%	4.219%
5	3.806	849	860	888	rBV	28195	84594	31.34%	3.496%
6	4.021	918	927	933	rBV5	1577	3247	1.20%	0.134%
7	4.253	983	999	1033	rVB	47077	123052	45.58%	5.085%
8	4.960	1205	1219	1244	rBV3	106909	269949	100.00%	11.156%
9	5.539	1388	1399	1432	rBV	98251	207015	76.69%	8.555%
10	5.992	1527	1540	1559	rBV	59822	123437	45.73%	5.101%
11	6.918	1818	1828	1853	rBV2	26449	52565	19.47%	2.172%
12	7.246	1919	1930	1958	rBV	126233	229165	84.89%	9.470%
13	7.561	2019	2028	2047	rBV	14485	28305	10.49%	1.170%
14	7.876	2115	2126	2138	rBV3	12604	22874	8.47%	0.945%
15	8.027	2164	2173	2224	rBV	131659	264185	97.86%	10.917%
16	8.786	2398	2409	2440	rBV	154006	255758	94.74%	10.569%
17	10.156	2824	2835	2855	rVB2	42566	67602	25.04%	2.794%
18	10.326	2876	2888	2900	rBV	24537	39987	14.81%	1.652%
19	11.188	3146	3156	3176	rBV	160714	251269	93.08%	10.384%
20	11.561	3262	3272	3294	rVB	128673	204164	75.63%	8.437%
21	12.194	3459	3469	3480	rVB	3180	4808	1.78%	0.199%




Sum of corrected areas: 2419855

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034077.D
Acq On : 08 Feb 2024 22:56
Operator : SY/MD
Sample : P1401-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

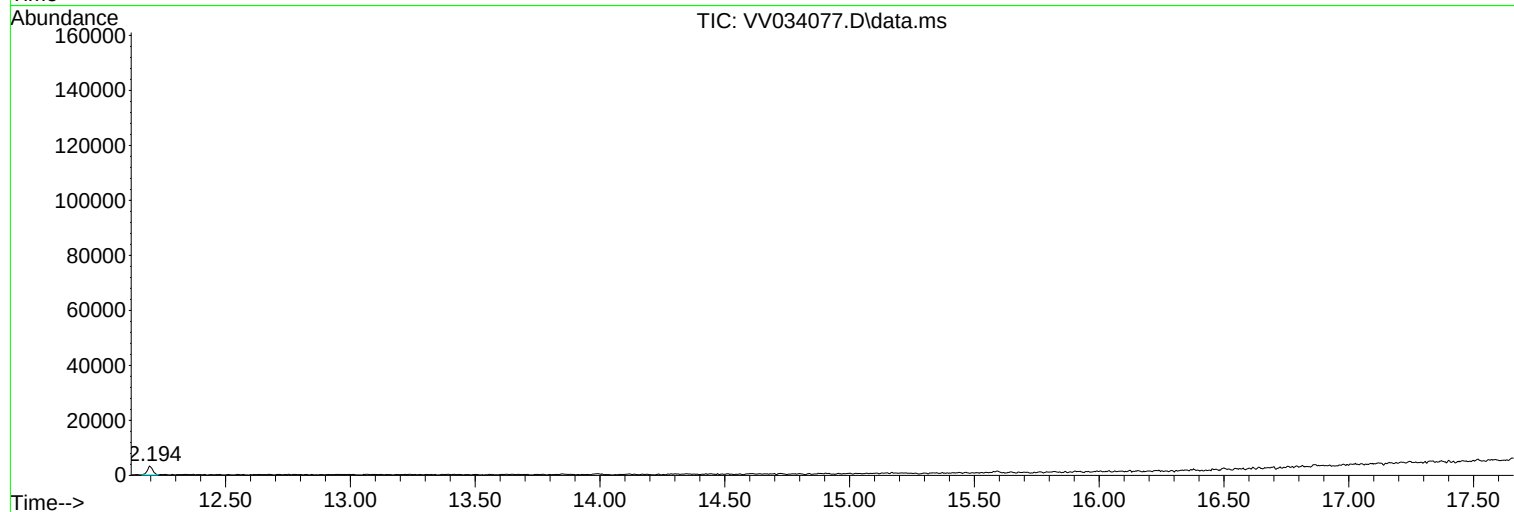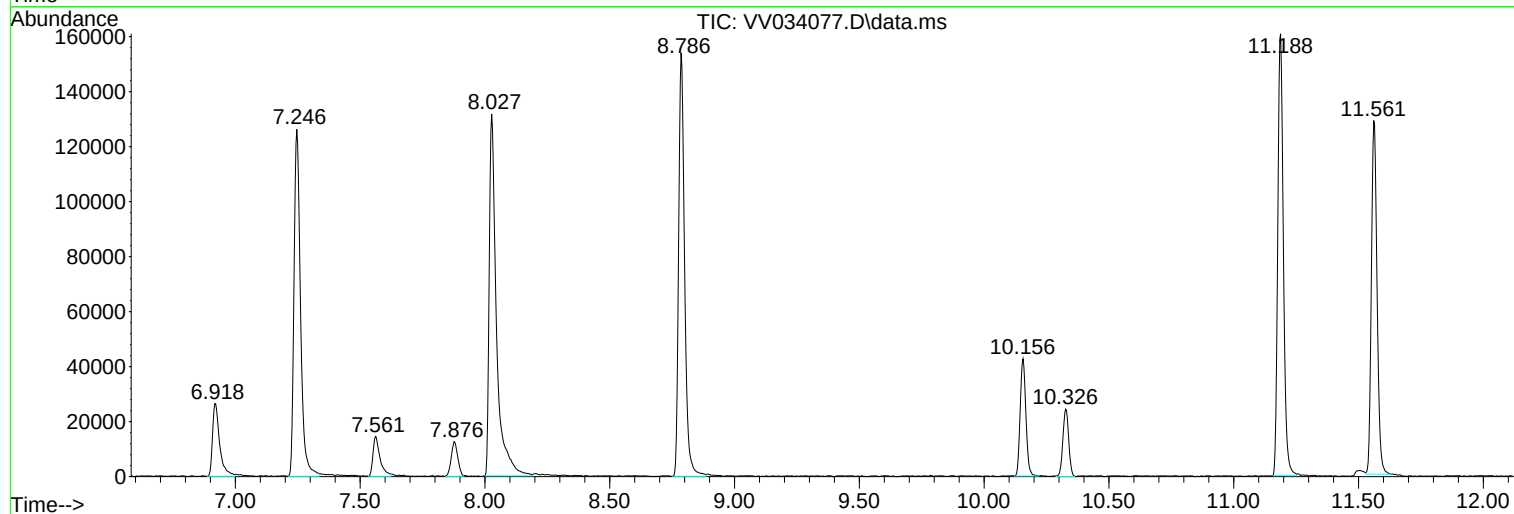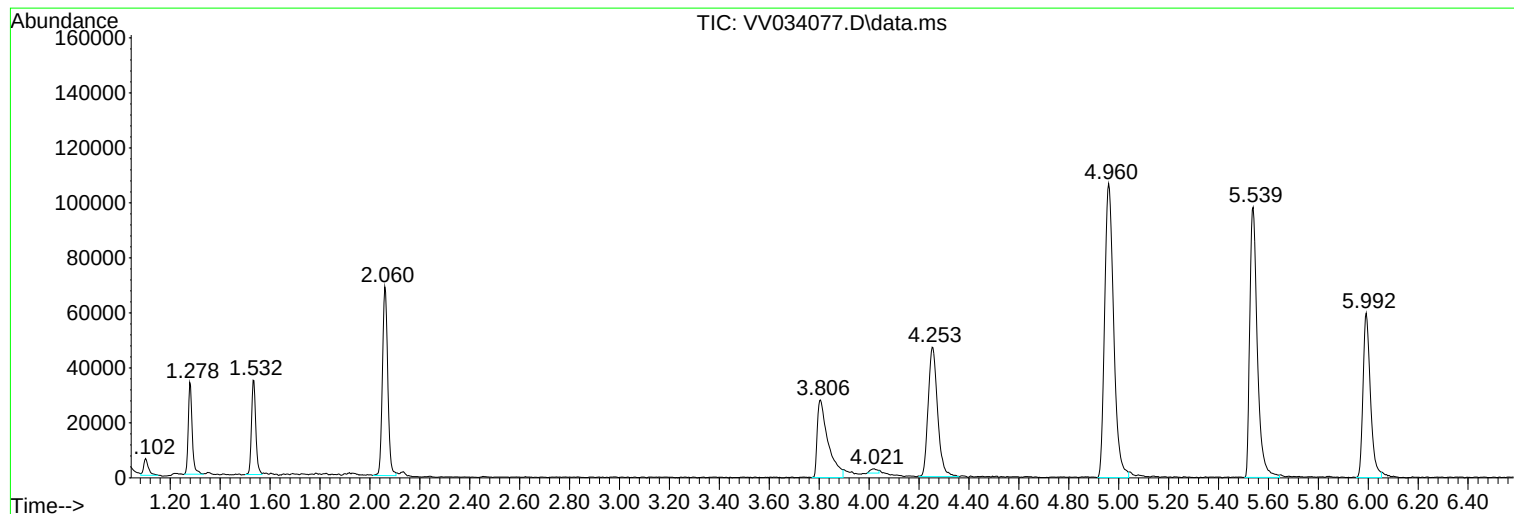

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034077.D
Acq On : 08 Feb 2024 22:56
Operator : SY/MD
Sample : P1401-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034077.D
Acq On : 08 Feb 2024 22:56
Operator : SY/MD
Sample : P1401-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc