

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
 Data File : VV034084.D
 Acq On : 09 Feb 2024 01:45
 Operator : SY/MD
 Sample : P1401-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034084.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	92	rVB	31678	34042	13.15%	1.425%
2	1.532	146	153	165	rVB	33166	38918	15.03%	1.630%
3	2.060	307	317	333	rBV	66682	97557	37.68%	4.085%
4	3.806	851	860	895	rBV	27319	86059	33.24%	3.603%
5	4.252	981	999	1023	rBV	45499	117688	45.45%	4.928%
6	4.960	1204	1219	1244	rBV3	102677	258926	100.00%	10.842%
7	5.539	1388	1399	1420	rBV	89926	187066	72.25%	7.833%
8	5.992	1529	1540	1571	rVB	58548	121608	46.97%	5.092%
9	6.918	1816	1828	1855	rBV2	25563	50254	19.41%	2.104%
10	7.246	1920	1930	1964	rBV	121732	223072	86.15%	9.341%
11	7.561	2016	2028	2045	rBV2	14005	26597	10.27%	1.114%
12	7.879	2112	2127	2143	rBV	30347	54525	21.06%	2.283%
13	8.027	2162	2173	2209	rBV	122750	246822	95.33%	10.335%
14	8.786	2399	2409	2432	rBV	141610	233915	90.34%	9.795%
15	10.156	2825	2835	2852	rBV	41482	65445	25.28%	2.740%
16	10.326	2877	2888	2901	rBV	55896	92756	35.82%	3.884%
17	11.188	3145	3156	3185	rBV	148580	238802	92.23%	9.999%
18	11.561	3262	3272	3296	rBV	123397	198981	76.85%	8.332%
19	12.197	3459	3470	3481	rVB2	9432	15176	5.86%	0.635%




Sum of corrected areas: 2388209

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034084.D
Acq On : 09 Feb 2024 01:45
Operator : SY/MD
Sample : P1401-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

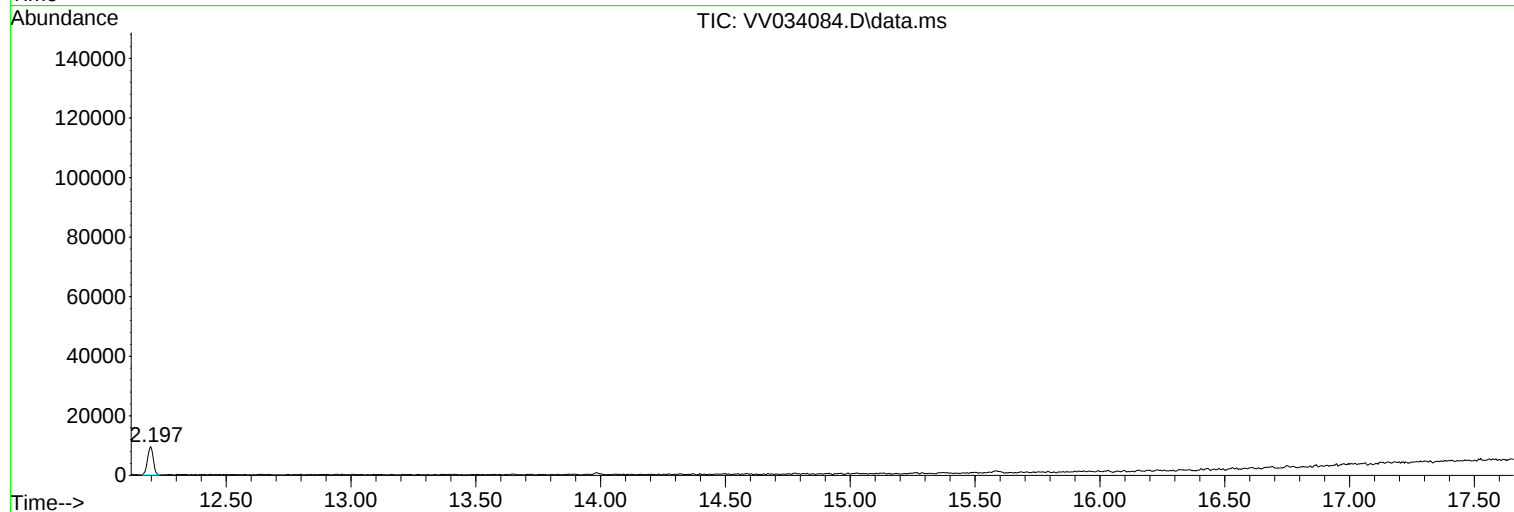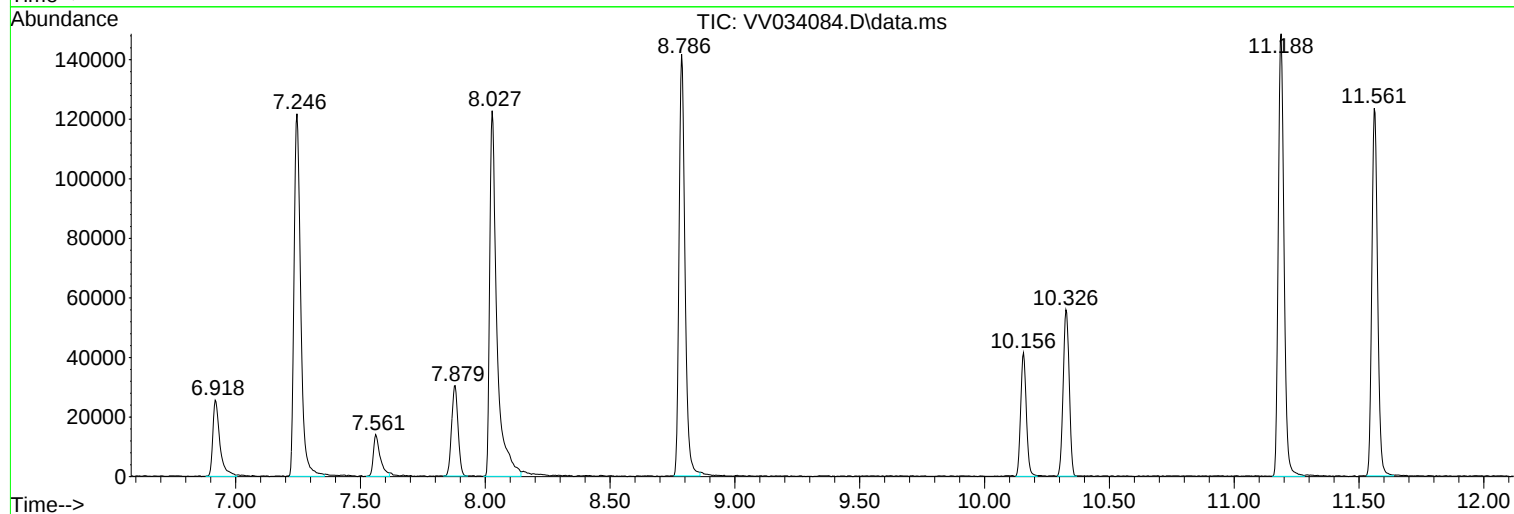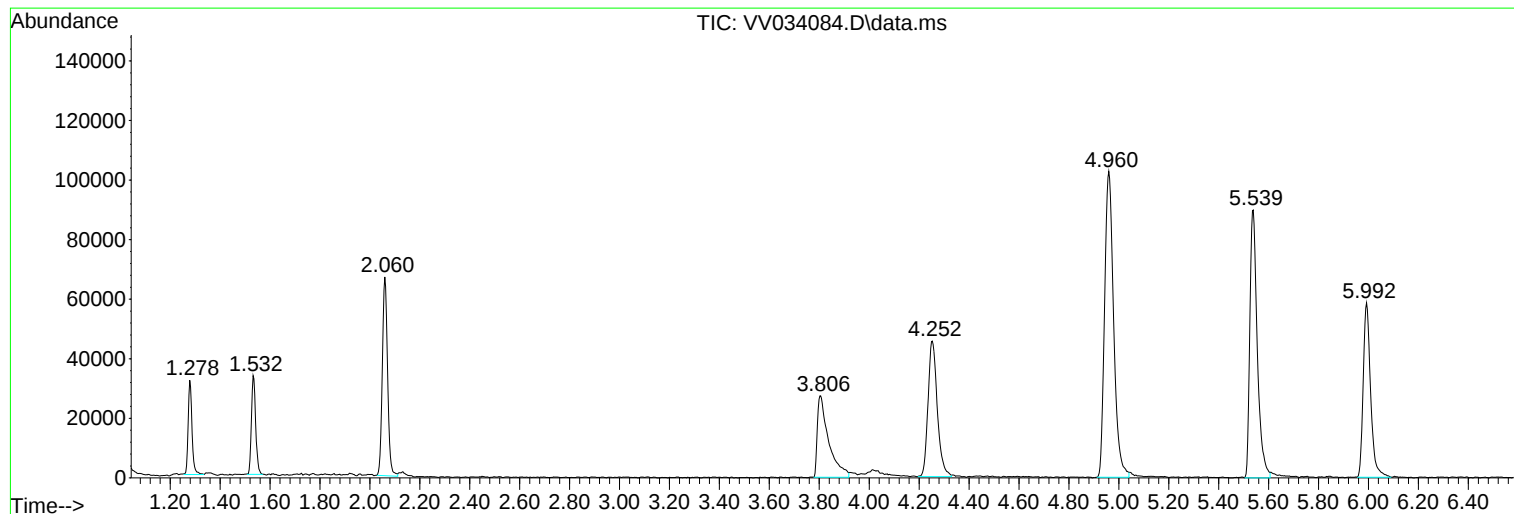

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034084.D
Acq On : 09 Feb 2024 01:45
Operator : SY/MD
Sample : P1401-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034084.D
Acq On : 09 Feb 2024 01:45
Operator : SY/MD
Sample : P1401-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc