

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
 Data File : VV034086.D
 Acq On : 09 Feb 2024 02:33
 Operator : SY/MD
 Sample : P1401-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034086.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	16	22	35	rVB2	1876	2813	1.09%	0.122%
2	1.278	67	74	91	rVB	31262	33208	12.92%	1.436%
3	1.532	146	153	166	rBV	32468	37957	14.76%	1.641%
4	2.059	306	317	329	rBV	63332	91409	35.55%	3.952%
5	3.809	850	861	896	rBV	25401	86167	33.52%	3.725%
6	4.018	917	926	933	rBV5	1556	3079	1.20%	0.133%
7	4.256	982	1000	1026	rBV	45574	120707	46.95%	5.218%
8	4.960	1205	1219	1246	rBV3	102831	257095	100.00%	11.114%
9	5.538	1388	1399	1429	rBV	93085	194553	75.67%	8.410%
10	5.992	1528	1540	1561	rBV2	56405	118057	45.92%	5.104%
11	6.921	1820	1829	1850	rBV2	24463	48586	18.90%	2.100%
12	7.246	1920	1930	1956	rBV	120695	218455	84.97%	9.444%
13	7.561	2020	2028	2050	rBV3	12831	26642	10.36%	1.152%
14	7.876	2115	2126	2148	rBV2	16064	34827	13.55%	1.506%
15	8.027	2164	2173	2220	rBV	119418	244592	95.14%	10.574%
16	8.786	2398	2409	2435	rBV	142423	237997	92.57%	10.289%
17	10.156	2824	2835	2850	rBV	39678	63101	24.54%	2.728%
18	10.329	2876	2889	2904	rVB	31062	50092	19.48%	2.165%
19	11.188	3146	3156	3171	rBV	149953	237549	92.40%	10.269%
20	11.561	3262	3272	3295	rBV	123747	197277	76.73%	8.528%
21	12.197	3459	3470	3480	rVB3	5556	9054	3.52%	0.391%




Sum of corrected areas: 2313217

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034086.D
Acq On : 09 Feb 2024 02:33
Operator : SY/MD
Sample : P1401-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

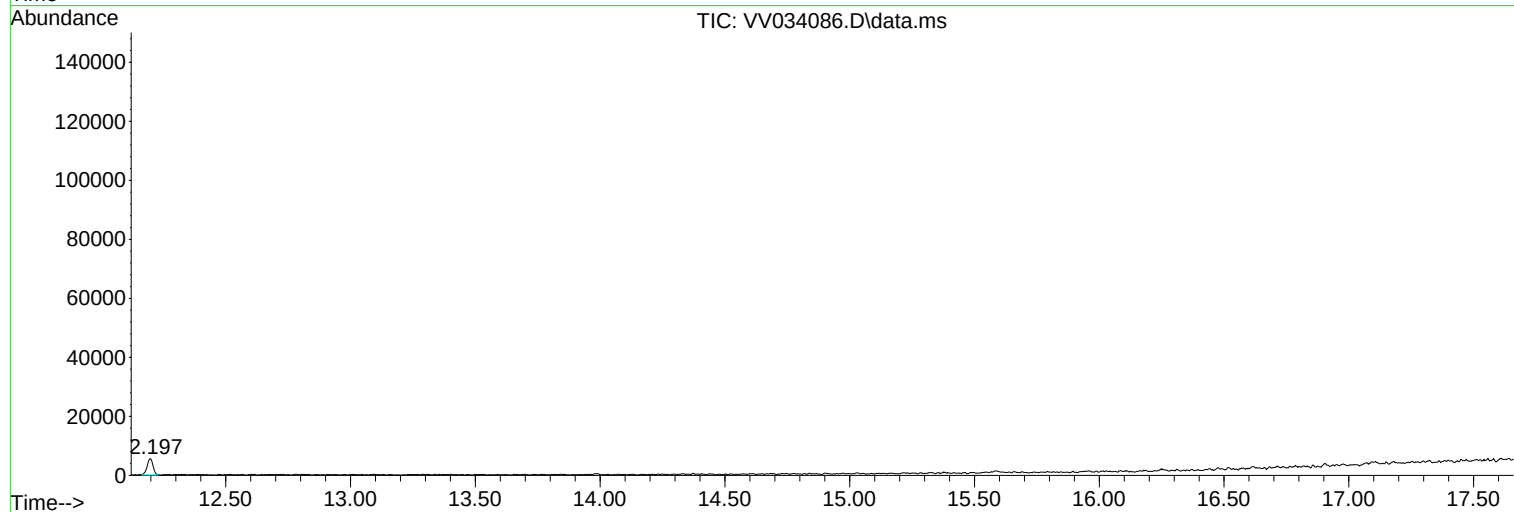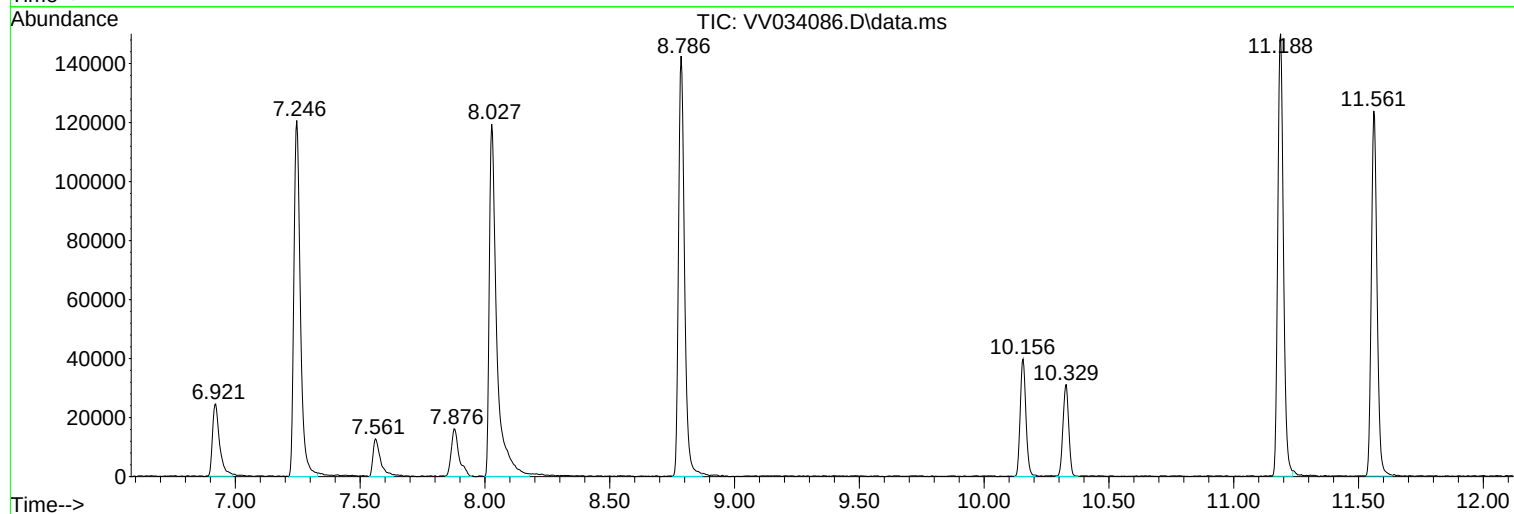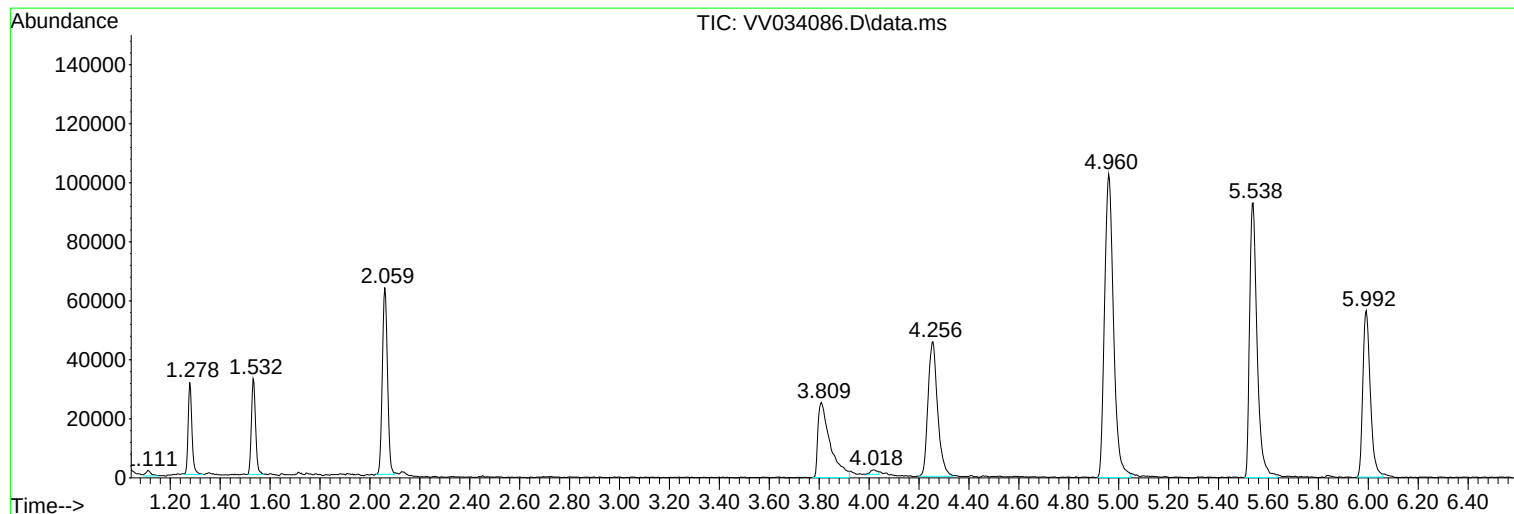

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034086.D
Acq On : 09 Feb 2024 02:33
Operator : SY/MD
Sample : P1401-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034086.D
Acq On : 09 Feb 2024 02:33
Operator : SY/MD
Sample : P1401-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------