

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
 Data File : VV034087.D
 Acq On : 09 Feb 2024 02:57
 Operator : SY/MD
 Sample : P1401-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034087.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	31440	33899	12.92%	1.488%
2	1.532	146	153	164	rBV	32631	37503	14.29%	1.647%
3	2.060	307	317	334	rBV	65688	95357	36.33%	4.187%
4	2.516	448	459	470	rBV2	9820	17893	6.82%	0.786%
5	3.809	853	861	899	rBV	23088	86963	33.13%	3.818%
6	4.011	914	924	937	rBV3	2530	6153	2.34%	0.270%
7	4.253	984	999	1020	rBV	46453	120362	45.86%	5.285%
8	4.960	1200	1219	1255	rBV2	102566	262473	100.00%	11.525%
9	5.535	1387	1398	1428	rBV	90389	189975	72.38%	8.341%
10	5.992	1527	1540	1564	rBV	56438	121114	46.14%	5.318%
11	6.921	1818	1829	1850	rBV2	24818	48097	18.32%	2.112%
12	7.246	1919	1930	1955	rBV	123741	219483	83.62%	9.637%
13	7.561	2020	2028	2048	rBV3	12986	25942	9.88%	1.139%
14	7.879	2114	2127	2139	rBV2	8405	15187	5.79%	0.667%
15	8.027	2164	2173	2208	rBV	118573	241820	92.13%	10.618%
16	8.786	2399	2409	2437	rBV	138414	230497	87.82%	10.121%
17	10.156	2824	2835	2851	rBV2	38657	63423	24.16%	2.785%
18	10.326	2877	2888	2901	rVB	18375	28556	10.88%	1.254%
19	11.188	3143	3156	3177	rBV	148636	231922	88.36%	10.183%
20	11.561	3262	3272	3290	rBV	123015	196891	75.01%	8.645%
21	12.198	3460	3470	3478	rBV3	2506	4011	1.53%	0.176%




Sum of corrected areas: 2277521

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034087.D
Acq On : 09 Feb 2024 02:57
Operator : SY/MD
Sample : P1401-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

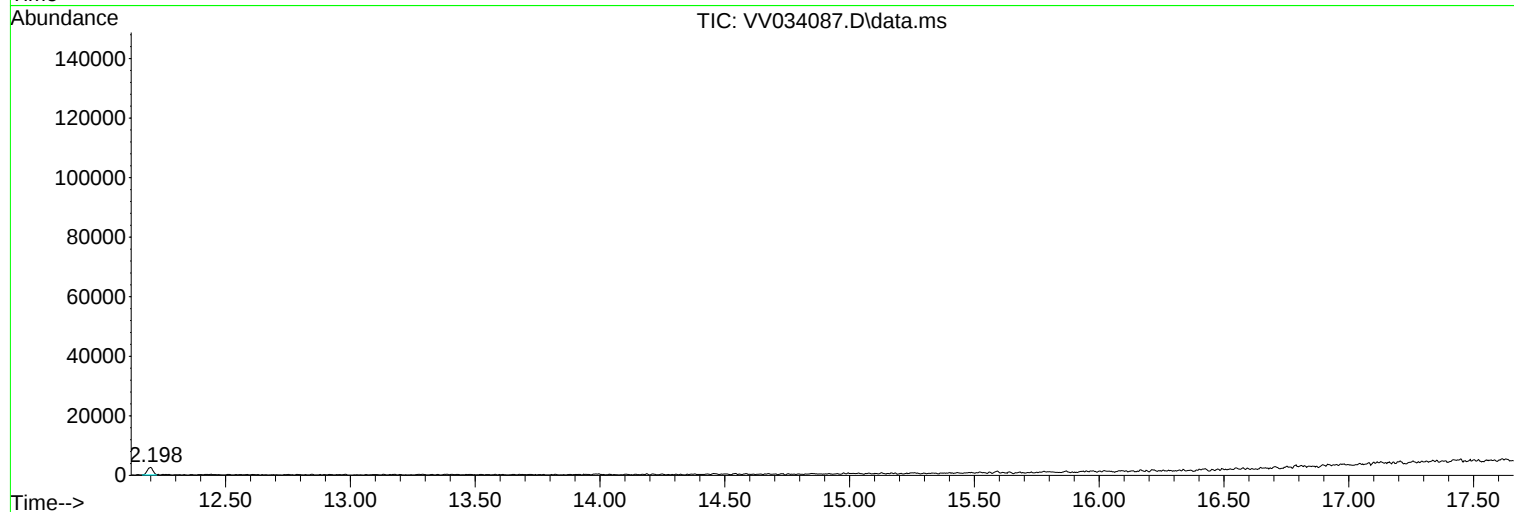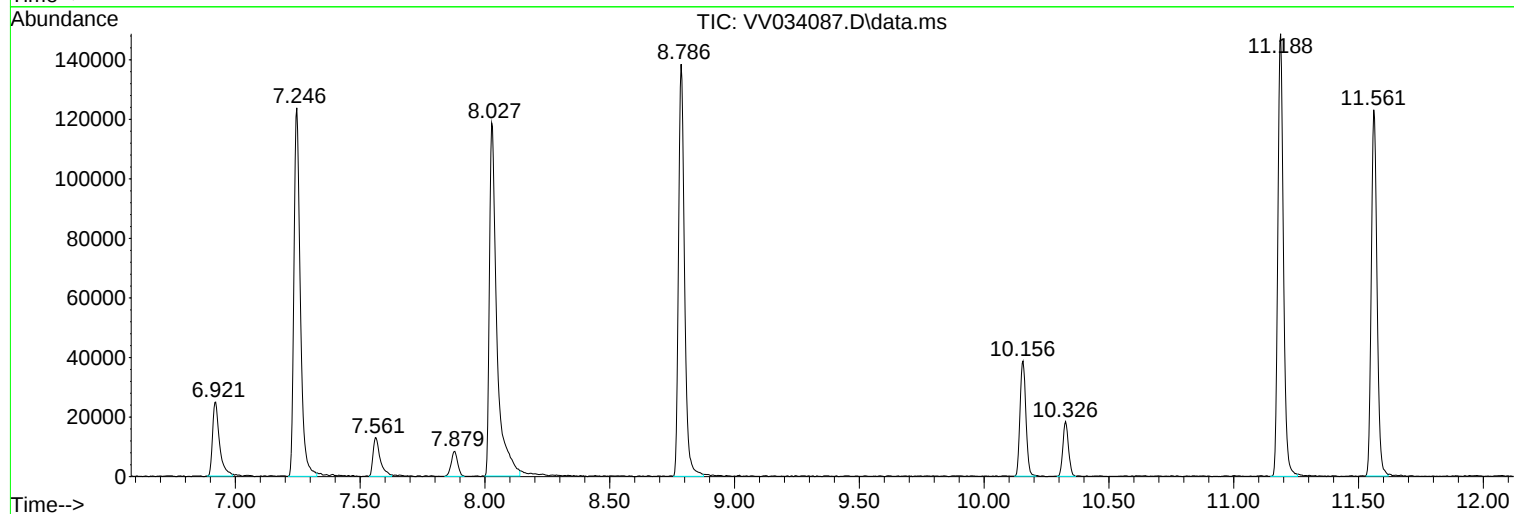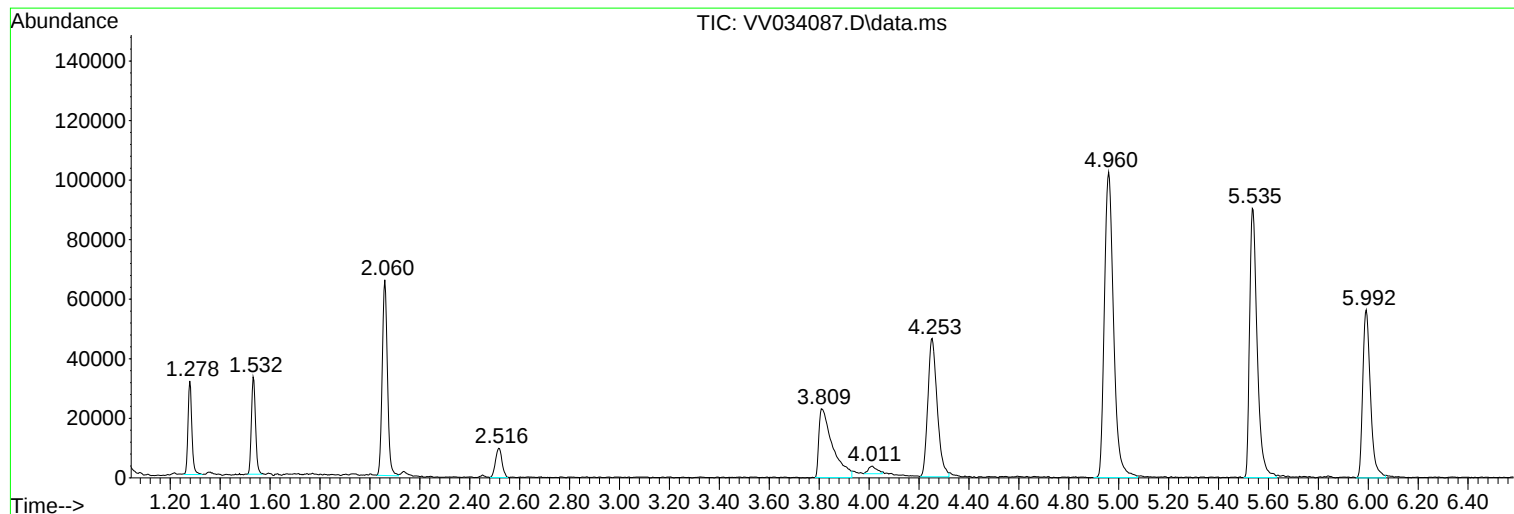

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034087.D
Acq On : 09 Feb 2024 02:57
Operator : SY/MD
Sample : P1401-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034087.D
Acq On : 09 Feb 2024 02:57
Operator : SY/MD
Sample : P1401-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc