

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
 Data File : VV034090.D
 Acq On : 09 Feb 2024 04:09
 Operator : SY/MD
 Sample : P1402-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV034090.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	65	74	88	rVB	32241	34117	1.53%	0.595%
2	1.532	143	153	164	rBV	32955	39061	1.76%	0.681%
3	2.063	308	318	333	rBV4	87612	145296	6.53%	2.533%
4	2.449	426	438	456	rVB	36231	60142	2.70%	1.048%
5	3.114	630	645	662	rBV	15685	33190	1.49%	0.579%
6	3.812	848	862	901	rBV2	267603	687453	30.89%	11.984%
7	4.252	984	999	1029	rBV	47236	130143	5.85%	2.269%
8	4.960	1203	1219	1251	rBV2	103151	264463	11.88%	4.610%
9	5.539	1388	1399	1434	rBV	90430	188181	8.46%	3.280%
10	5.831	1476	1490	1522	rBV	1140592	2225522	100.00%	38.796%
11	5.992	1528	1540	1561	rVB2	57535	117487	5.28%	2.048%
12	6.918	1820	1828	1853	rBV2	25042	47876	2.15%	0.835%
13	7.246	1919	1930	1954	rBV	124733	220530	9.91%	3.844%
14	7.561	2020	2028	2049	rBV	13288	25973	1.17%	0.453%
15	7.905	2115	2135	2164	rBV	320674	542548	24.38%	9.458%
16	8.027	2164	2173	2208	rBV	123479	241178	10.84%	4.204%
17	8.786	2398	2409	2437	rBV	134649	227746	10.23%	3.970%
18	10.156	2825	2835	2850	rBV	39844	63985	2.88%	1.115%
19	11.188	3146	3156	3179	rBV	147421	235537	10.58%	4.106%
20	11.561	3262	3272	3294	rBV	128623	205990	9.26%	3.591%




Sum of corrected areas: 5736418

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034090.D
Acq On : 09 Feb 2024 04:09
Operator : SY/MD
Sample : P1402-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

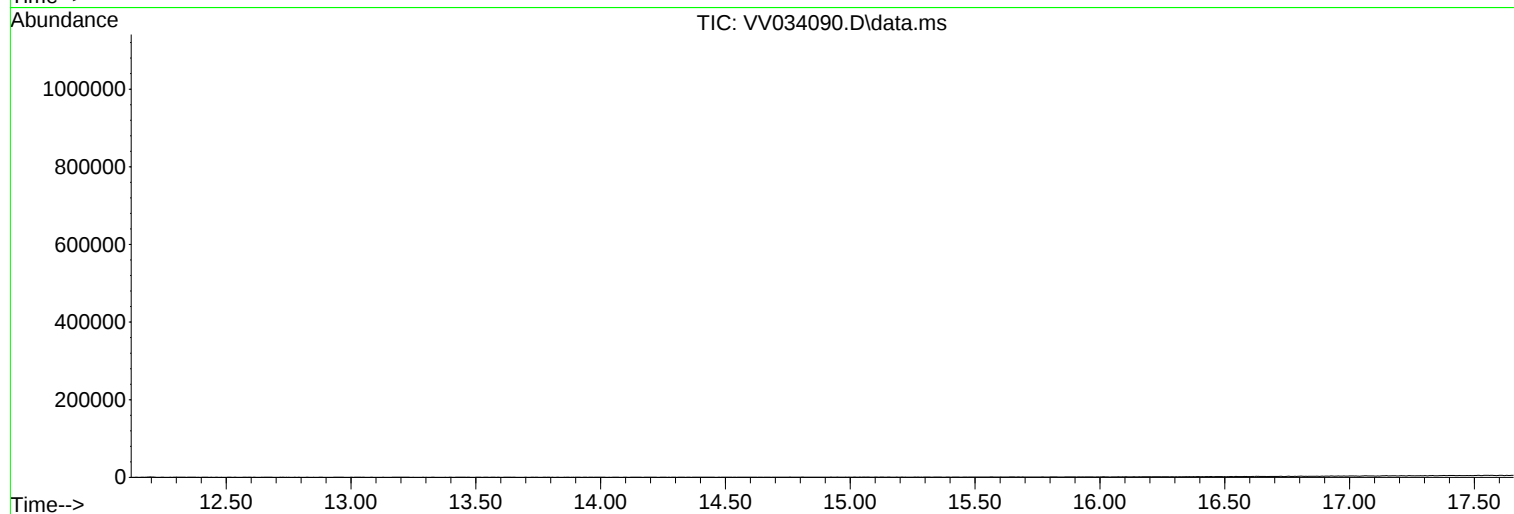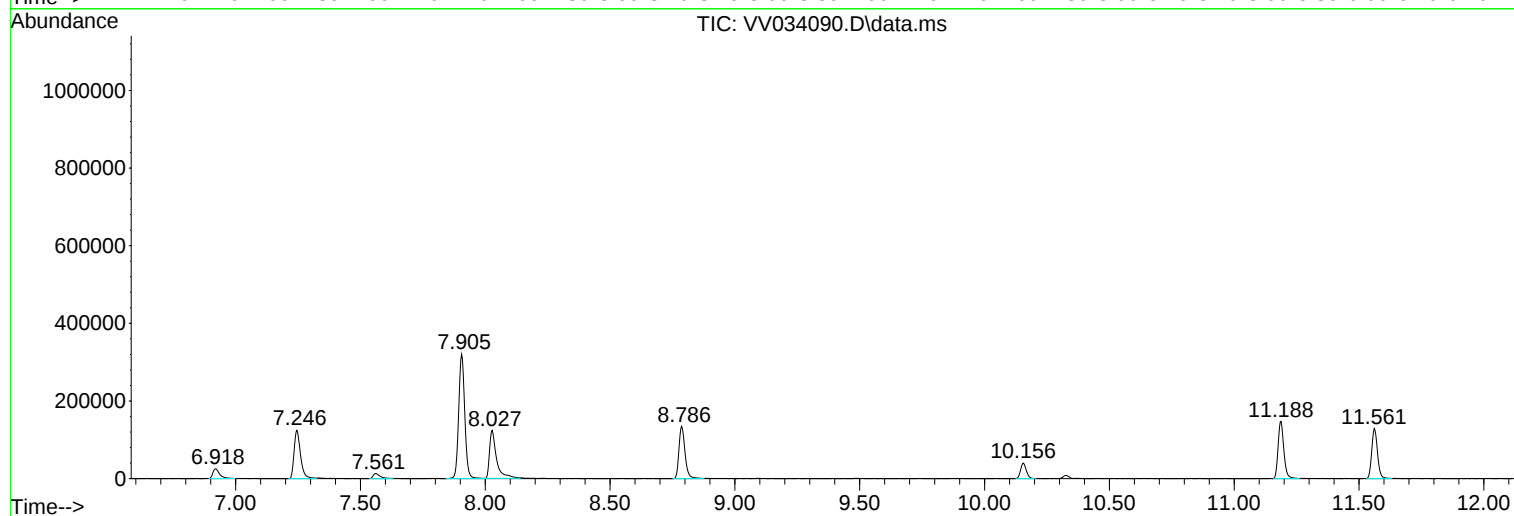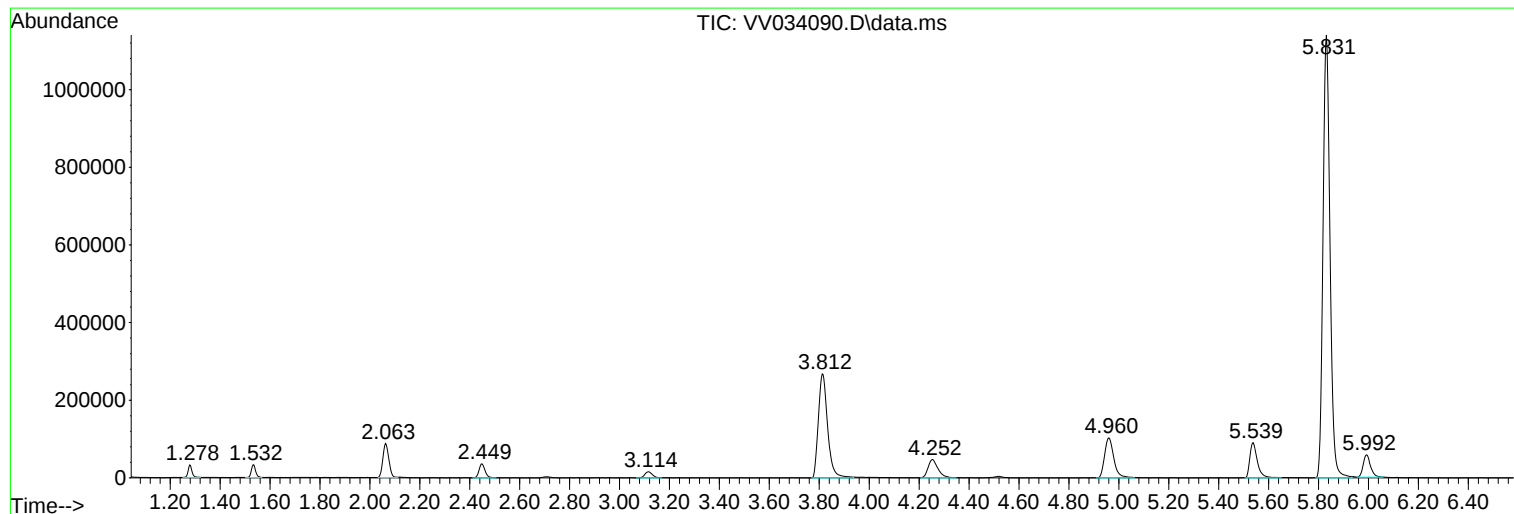

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034090.D
Acq On : 09 Feb 2024 04:09
Operator : SY/MD
Sample : P1402-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034090.D
Acq On : 09 Feb 2024 04:09
Operator : SY/MD
Sample : P1402-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------