

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
 Data File : VV034092.D
 Acq On : 09 Feb 2024 04:57
 Operator : SY/MD
 Sample : P1402-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV034092.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rBV	29693	31514	12.95%	1.241%
2	1.532	146	153	163	rBV	31316	36575	15.03%	1.440%
3	2.063	307	318	331	rBV2	86761	143272	58.86%	5.640%
4	2.706	506	518	540	rBV2	22332	46055	18.92%	1.813%
5	3.117	637	646	657	rBV4	2100	4263	1.75%	0.168%
6	3.805	850	860	885	rBV3	31393	101739	41.79%	4.005%
7	4.252	984	999	1029	rBV	43780	116341	47.79%	4.580%
8	4.960	1205	1219	1247	rBV2	95793	243424	100.00%	9.583%
9	5.535	1388	1398	1428	rBV	89283	183381	75.33%	7.219%
10	5.838	1479	1492	1520	rBV	41342	87629	36.00%	3.450%
11	5.992	1528	1540	1573	rBV2	54346	113353	46.57%	4.462%
12	6.918	1817	1828	1856	rBV2	23375	47211	19.39%	1.859%
13	7.246	1919	1930	1956	rBV2	113987	206878	84.99%	8.144%
14	7.561	2020	2028	2049	rBV3	12523	23919	9.83%	0.942%
15	7.905	2121	2135	2157	rVB	114552	195775	80.43%	7.707%
16	8.027	2162	2173	2215	rBV	116479	237411	97.53%	9.346%
17	8.786	2399	2409	2436	rBV	138029	231238	94.99%	9.103%
18	10.152	2825	2834	2852	rBV2	36794	61024	25.07%	2.402%
19	10.326	2882	2888	2896	rVB4	2092	2763	1.14%	0.109%
20	11.188	3145	3156	3180	rBV	150748	235770	96.86%	9.282%
21	11.561	3262	3272	3296	rBV	120535	190654	78.32%	7.506%




Sum of corrected areas: 2540189

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034092.D
Acq On : 09 Feb 2024 04:57
Operator : SY/MD
Sample : P1402-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

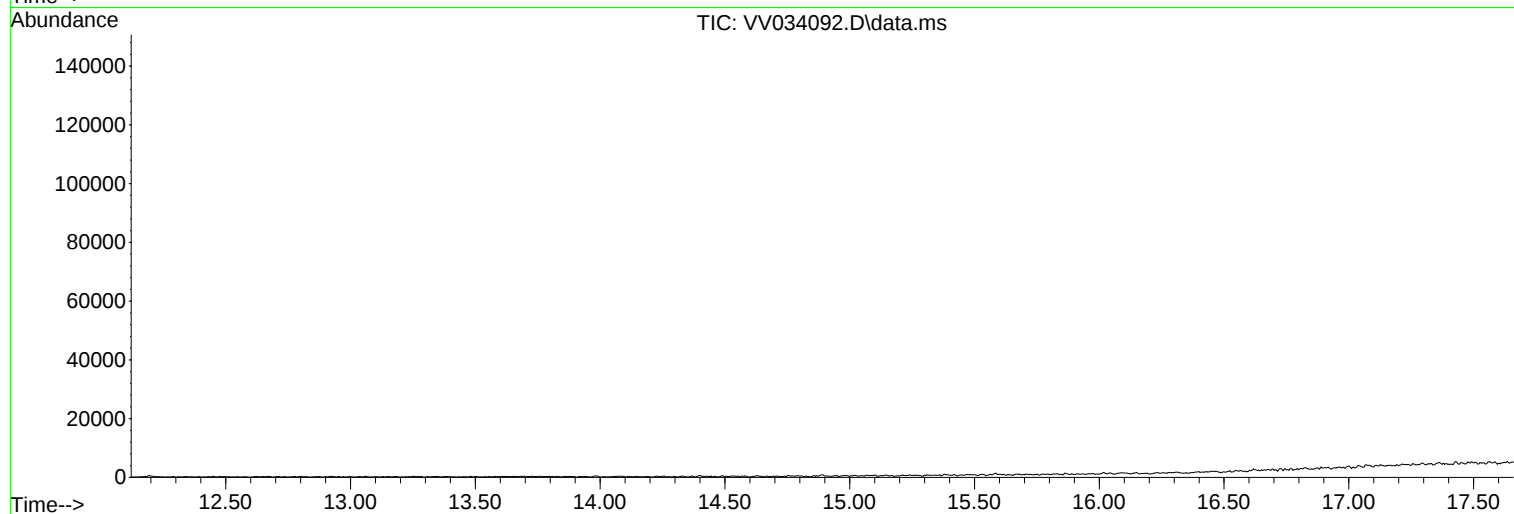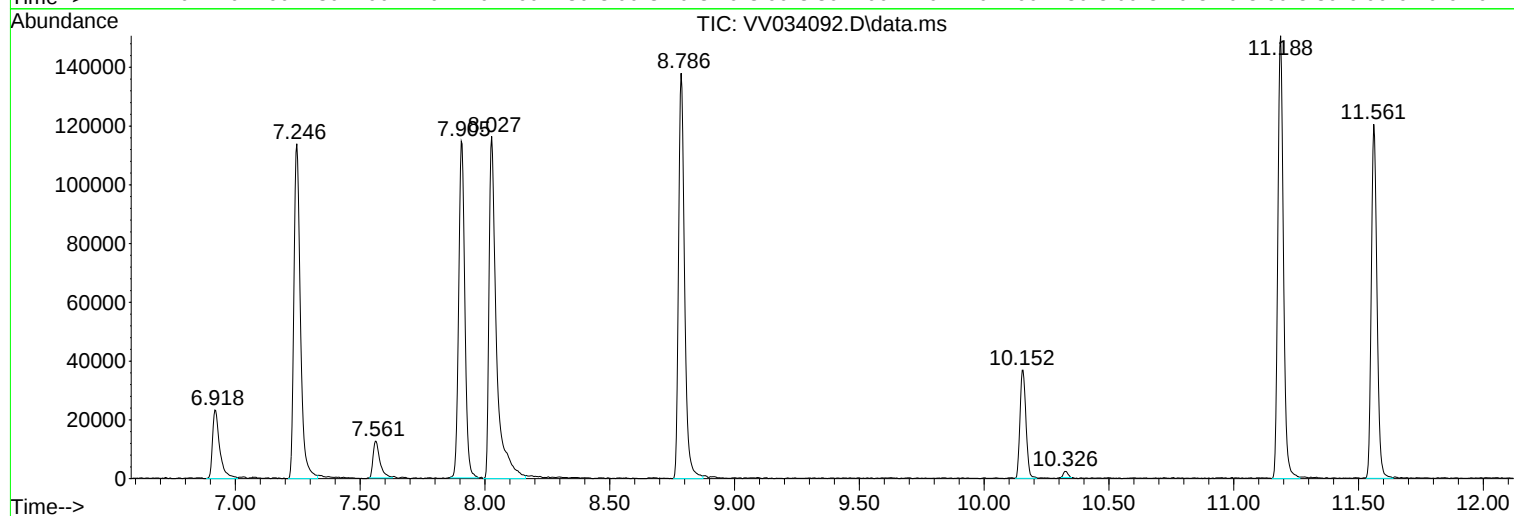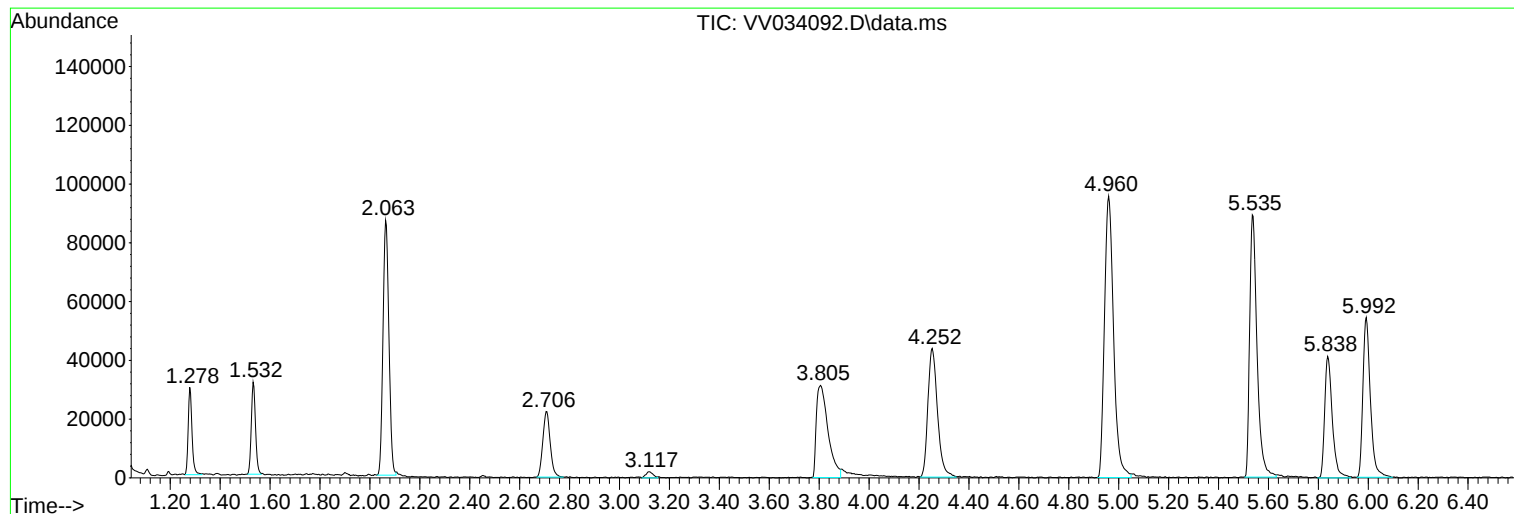

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034092.D
Acq On : 09 Feb 2024 04:57
Operator : SY/MD
Sample : P1402-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020824\
Data File : VV034092.D
Acq On : 09 Feb 2024 04:57
Operator : SY/MD
Sample : P1402-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc