
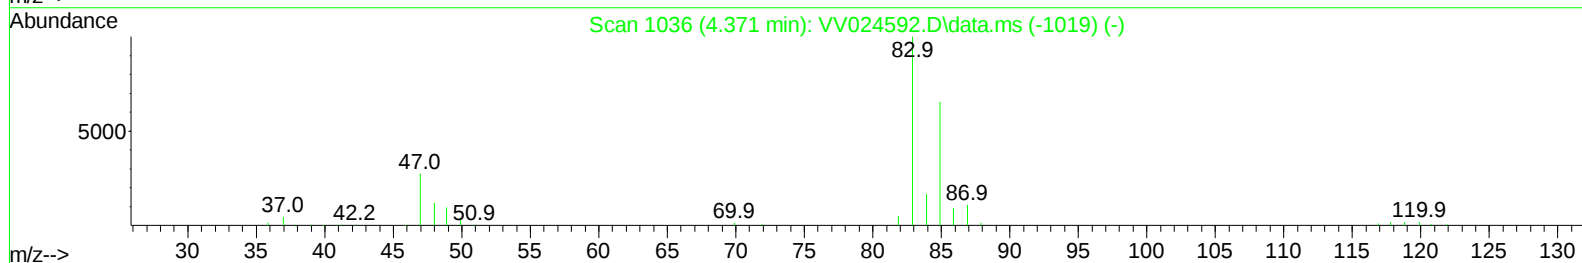
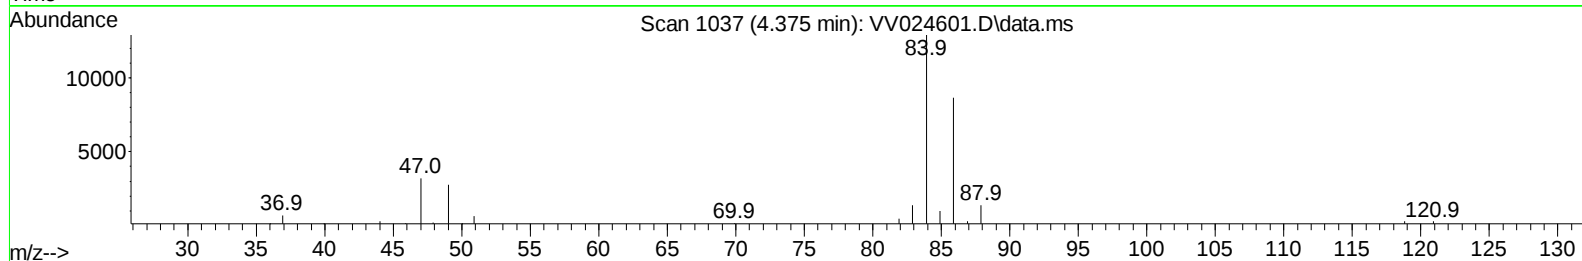


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024601.D
Acq On : 11 Feb 2022 14:04
Operator : SY/MD
Sample : N1476-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Feb 12 03:43:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Feb 12 03:41:27 2022
Response via : Initial Calibration

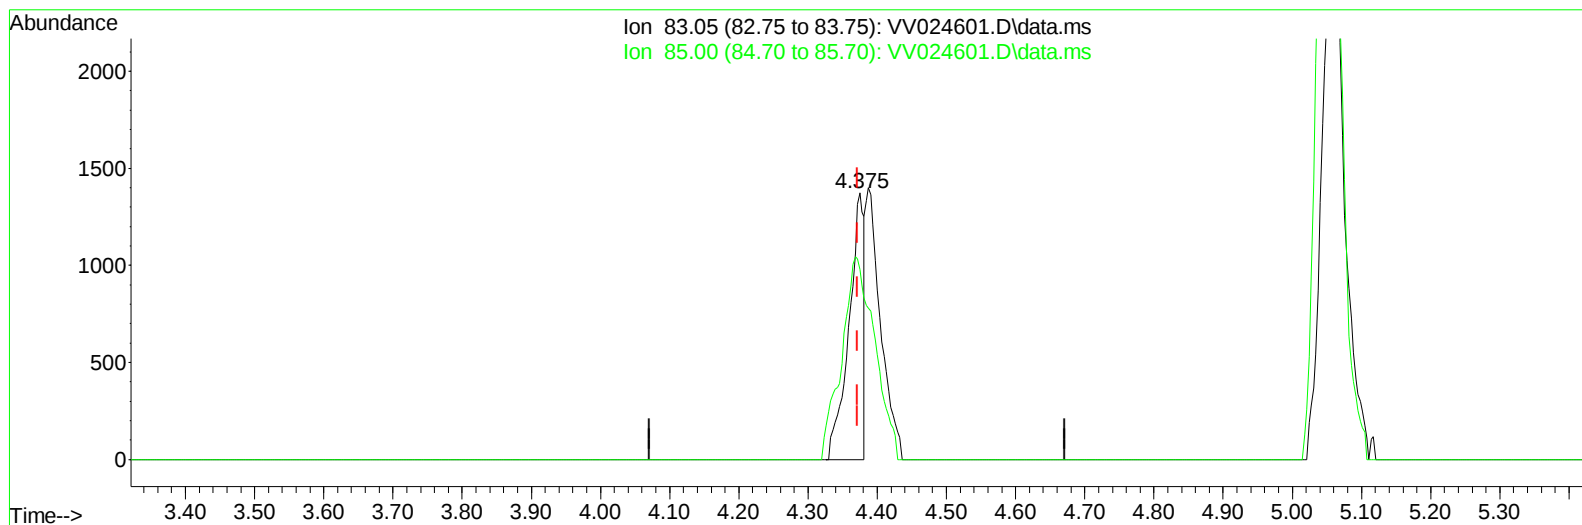

TIC: VV024601.D\data.ms

(25) Chloroform (T)

4.375min (+ 0.003) 0.10 ug/L

response 2094

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	64.60	71.36
0.00	0.00	0.00
0.00	0.00	0.00