


Abundance Scan 1583 (6.130 min): VV024617.D\data.ms (-15735)

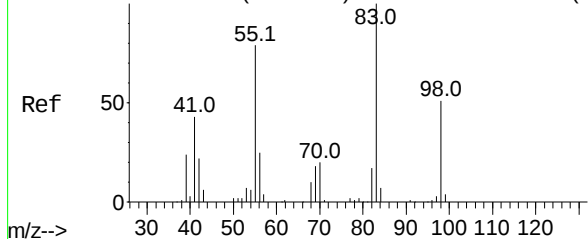

Methylcyclohexane

Concen: 0.558 ug/L

RT: 6.072 min Scan# 1565

Delta R.T. -0.058 min

Lab File: VV024623.D

Acq: 11 Feb 2022 23:45

Instrument :

MSVOA_V

ClientSampleId :



Tgt Ion: 83 Resp: 11639

Ion Ratio Lower Upper


83 100

55 0.0 60.2 90.2#


98 0.7 41.0 61.4#

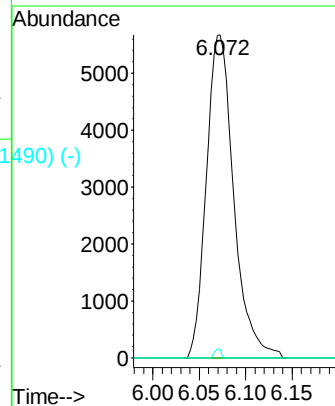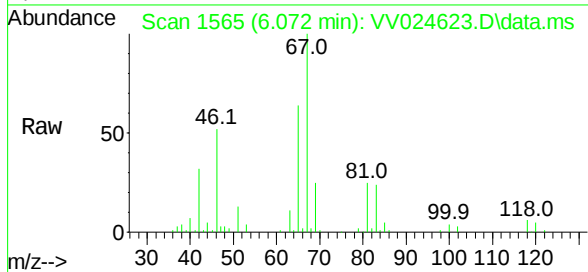

Abundance Scan 1565 (6.072 min): VV024623.D\data.ms (-1490)

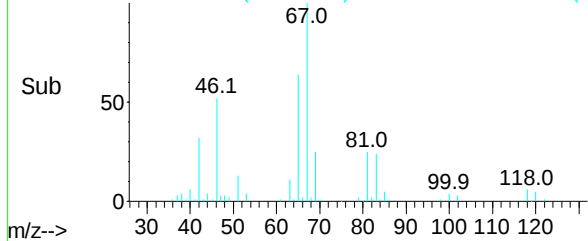

Abundance Scan 1597 (6.175 min): VV024617.D\data.ms (-15737)

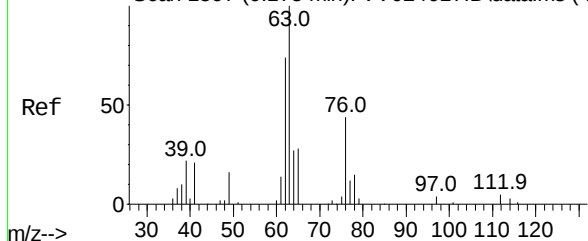

1,2-Dichloropropane

Concen: 0.520 ug/L

RT: 6.069 min Scan# 1564

Delta R.T. -0.106 min

Lab File: VV024623.D



Acq: 11 Feb 2022 23:45

Tgt Ion: 63 Resp: 5772

Ion Ratio Lower Upper

63 100

112 0.0 4.3 6.5#

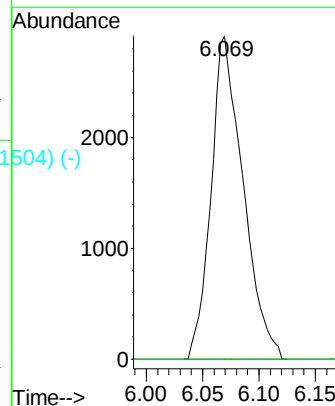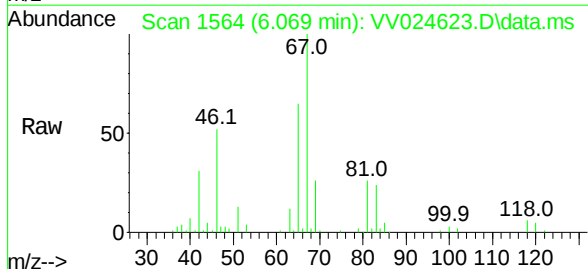

Abundance Scan 1564 (6.069 min): VV024623.D\data.ms (-1504)

