




Abundance Scan 1862 (7.027 min): VV024617.D\data.ms (-18429)

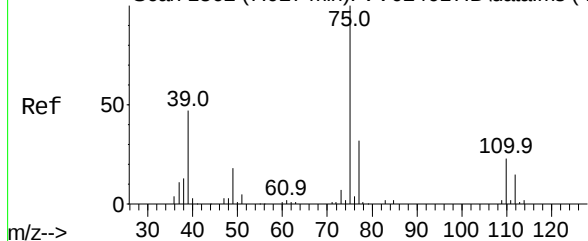


cis-1,3-Dichloropropene
Concen: 0.075 ug/L
RT: 6.989 min Scan# 2159
Delta R.T. -0.039 min
Lab File: VV024623.D
Acq: 11 Feb 2022 23:45

Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion: 75 Resp: 1263
Ion Ratio Lower Upper
75 100
77 47.5 22.0 41.0#

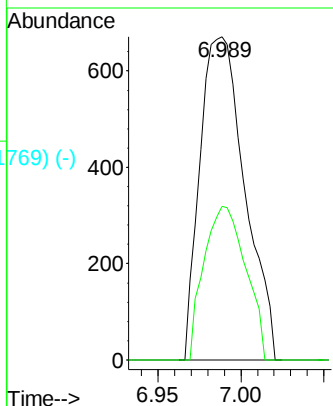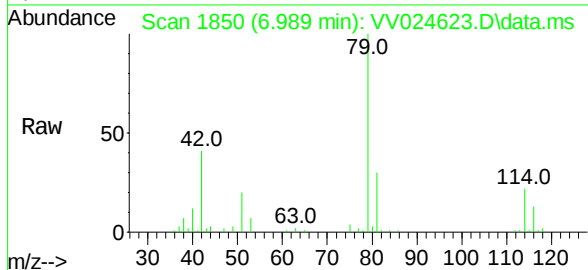

Abundance Scan 1850 (6.989 min): VV024623.D\data.ms (-1769)


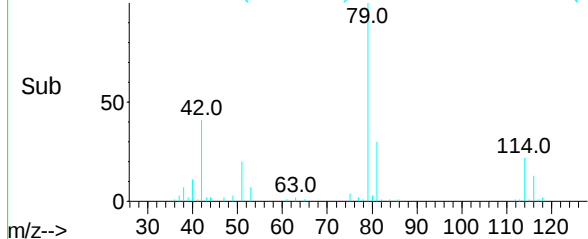


Abundance Scan 2241 (8.246 min): VV024617.D\data.ms (-22289)

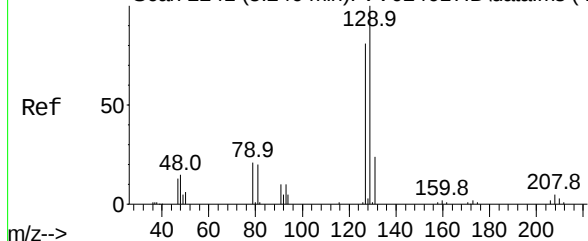

Dibromochloromethane
Concen: 0.030 ug/L
RT: 7.982 min Scan# 2159
Delta R.T. -0.264 min
Lab File: VV024623.D
Acq: 11 Feb 2022 23:45

Tgt Ion:129 Resp: 258
Ion Ratio Lower Upper
129 100
127 0.0 53.5 99.3#

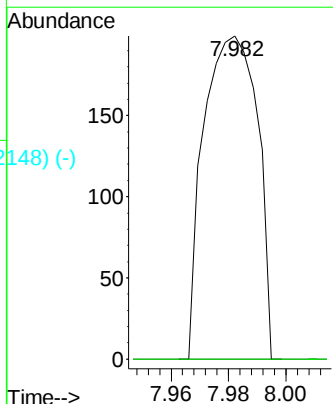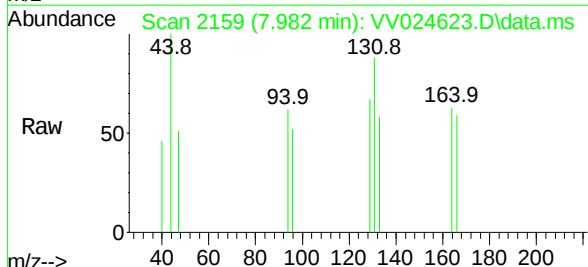

Abundance Scan 2159 (7.982 min): VV024623.D\data.ms (-2148)

