


Abundance Scan 2871 (10.272 min): VV024617.D\data.ms (-2861) (-)

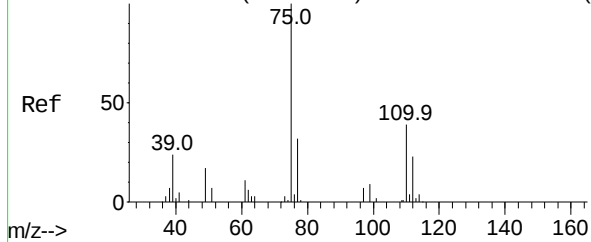

1,2,3-Trichloropropane

Concen: 1.410 ug/L

RT: 11.249 min Scan#

Delta R.T. 0.977 min

Lab File: VV024623.D


Acq: 11 Feb 2022 23:45

Instrument :

MSVOA_V

ClientSampleId :

Abundance Scan 3175 (11.249 min): VV024623.D\data.ms

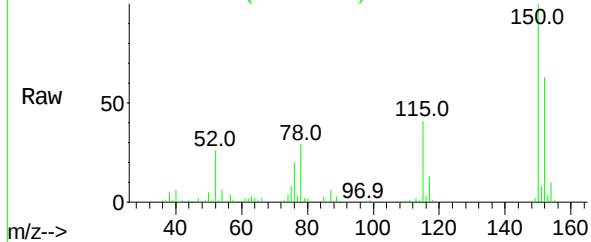


Tgt Ion: 75 Resp: 7935

Ion Ratio Lower Upper

75 100

77 34.0 26.4 39.6

110 2.4 34.2 51.2#

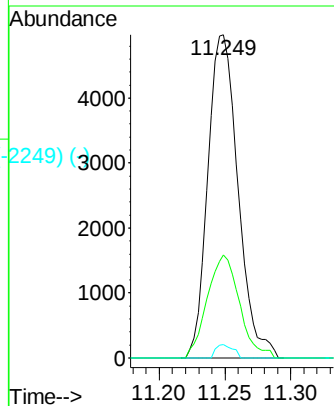

Abundance Scan 3175 (11.249 min): VV024623.D\data.ms (-2249) (-)

