

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021122\
 Data File : VW024602.D
 Acq On : 11 Feb 2022 14:28
 Operator : SY/MD
 Sample : VIBLK254
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK254

Quant Time: Feb 12 03:43:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Feb 12 03:41:27 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	123908	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	123609	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	62121	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	41313	3.978	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	79.600%	
7) Chloroethane-d5	1.571	69	38877	4.428	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	88.600%	
11) 1,1-Dichloroethene-d2	2.111	63	66441	2.924	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	58.400%#	
20) 2-Butanone-d5	3.892	46	92891	53.874	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	107.740%	
24) Chloroform-d	4.352	84	84202	4.606	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.200%	
26) 1,2-Dichloroethane-d4	5.034	65	41106	4.956	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	99.200%	
32) Benzene-d6	5.053	84	171778	4.898	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.000%	
36) 1,2-Dichloropropane-d6	6.069	67	52158	4.782	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	95.600%	
41) Toluene-d8	7.317	98	152919	4.675	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	93.400%	
43) trans-1,3-Dichloroprop...	7.625	79	19778	4.490	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	89.800%	
46) 2-Hexanone-d5	8.088	63	75880	48.893	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	97.780%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31427	4.839	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	96.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	48570	4.850	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	97.000%	
Target Compounds					Qvalue	
25) Chloroform	4.378	83	2489	0.109	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024602.D
Acq On : 11 Feb 2022 14:28
Operator : SY/MD
Sample : VIBLK254
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK254

Quant Time: Feb 12 03:43:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Feb 12 03:41:27 2022
Response via : Initial Calibration

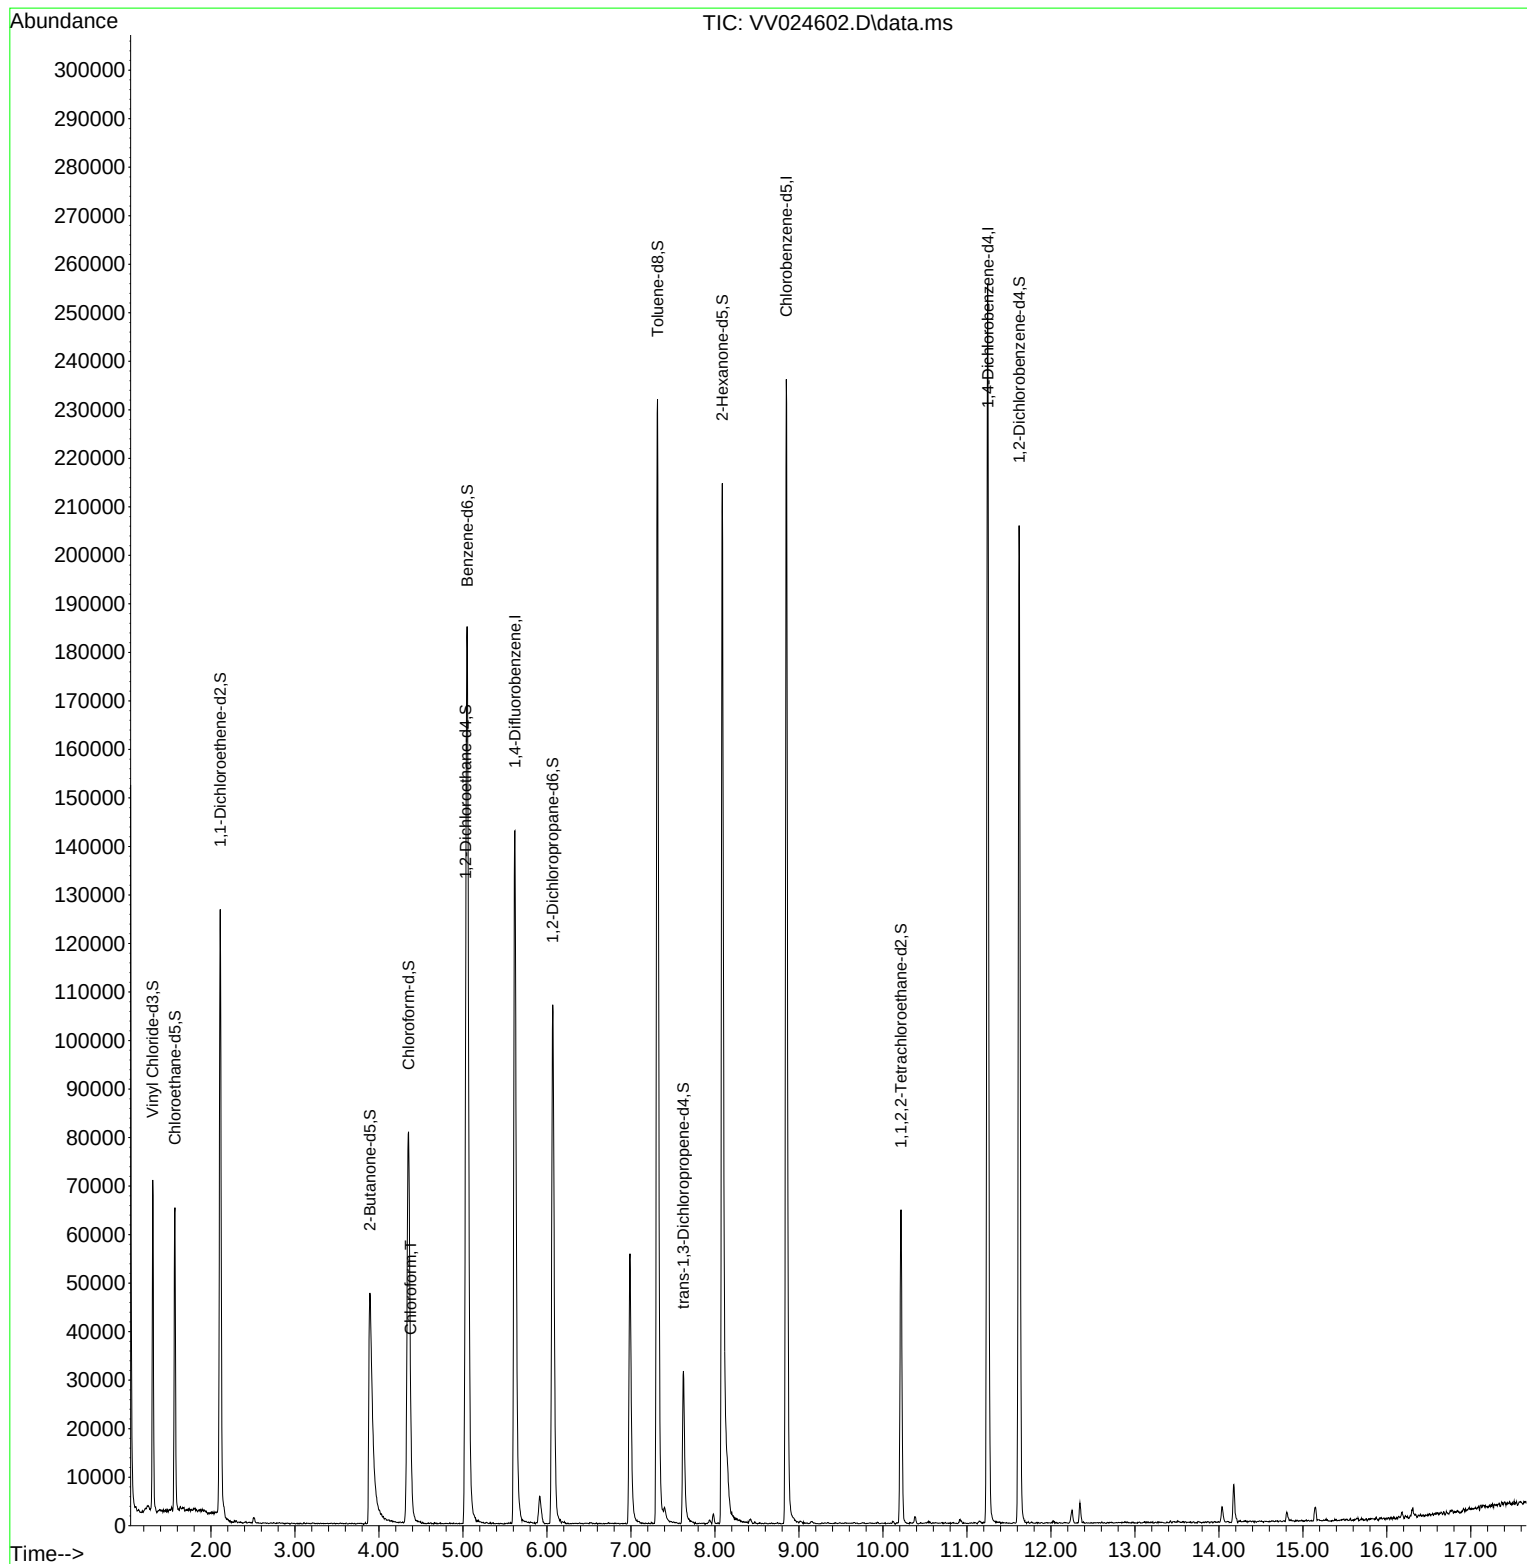

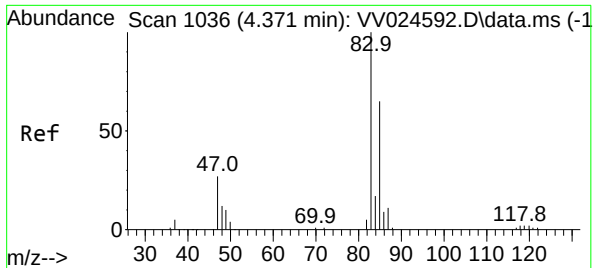

#25
 Chloroform
 Concen: 0.109 ug/L
 RT: 4.378 min Scan# 10
 Delta R.T. 0.007 min
 Lab File: VV024602.D
 Acq: 11 Feb 2022 14:28

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK254

Tgt Ion: 83 Resp: 2489
 Ion Ratio Lower Upper
 83 100
 85 62.4 45.2 84.0

