

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW021122\  
 Data File : VW024610.D  
 Acq On : 11 Feb 2022 17:45  
 Operator : SY/MD  
 Sample : N1479-04  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 21 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 GBCW2

Quant Time: Feb 12 03:45:46 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR020922WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Feb 12 03:41:27 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units  | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|--------|----------|
| -----                         |        |       |          |          |        |          |
| Internal Standards            |        |       |          |          |        |          |
| 1) 1,4-Difluorobenzene        | 5.619  | 114   | 123265   | 5.000    | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 8.850  | 117   | 123000   | 5.000    | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.249 | 152   | 60969    | 5.000    | ug/L   | 0.00     |
|                               |        |       |          |          |        |          |
| System Monitoring Compounds   |        |       |          |          |        |          |
| 4) Vinyl Chloride-d3          | 1.307  | 65    | 43772    | 4.236    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =      | 84.800%  |
| 7) Chloroethane-d5            | 1.568  | 69    | 41541    | 4.756    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =      | 95.200%  |
| 11) 1,1-Dichloroethene-d2     | 2.108  | 63    | 70564    | 3.122    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =      | 62.400%  |
| 20) 2-Butanone-d5             | 3.892  | 46    | 92918    | 54.171   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =      | 108.340% |
| 24) Chloroform-d              | 4.349  | 84    | 84465    | 4.645    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 92.800%  |
| 26) 1,2-Dichloroethane-d4     | 5.034  | 65    | 41381    | 5.015    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 100.200% |
| 32) Benzene-d6                | 5.050  | 84    | 169472   | 4.856    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 97.200%  |
| 36) 1,2-Dichloropropane-d6    | 6.069  | 67    | 53275    | 4.908    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =      | 98.200%  |
| 41) Toluene-d8                | 7.317  | 98    | 155403   | 4.774    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 95.400%  |
| 43) trans-1,3-Dichloroprop... | 7.625  | 79    | 18774    | 4.283    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =      | 85.600%  |
| 46) 2-Hexanone-d5             | 8.088  | 63    | 76050    | 49.245   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =      | 98.480%  |
| 56) 1,1,2,2-Tetrachloroeth... | 10.217 | 84    | 31335    | 4.849    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =      | 97.000%  |
| 66) 1,2-Dichlorobenzene-d4    | 11.622 | 152   | 49221    | 5.008    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =      | 100.200% |
|                               |        |       |          |          |        |          |
| Target Compounds              |        |       |          |          | Qvalue |          |
| 25) Chloroform                | 4.372  | 83    | 1629     | 0.072    | ug/L   | 94       |
| -----                         |        |       |          |          |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV021122\  
Data File : VV024610.D  
Acq On : 11 Feb 2022 17:45  
Operator : SY/MD  
Sample : N1479-04  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
GBCW2

Quant Time: Feb 12 03:45:46 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR020922WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Sat Feb 12 03:41:27 2022  
Response via : Initial Calibration

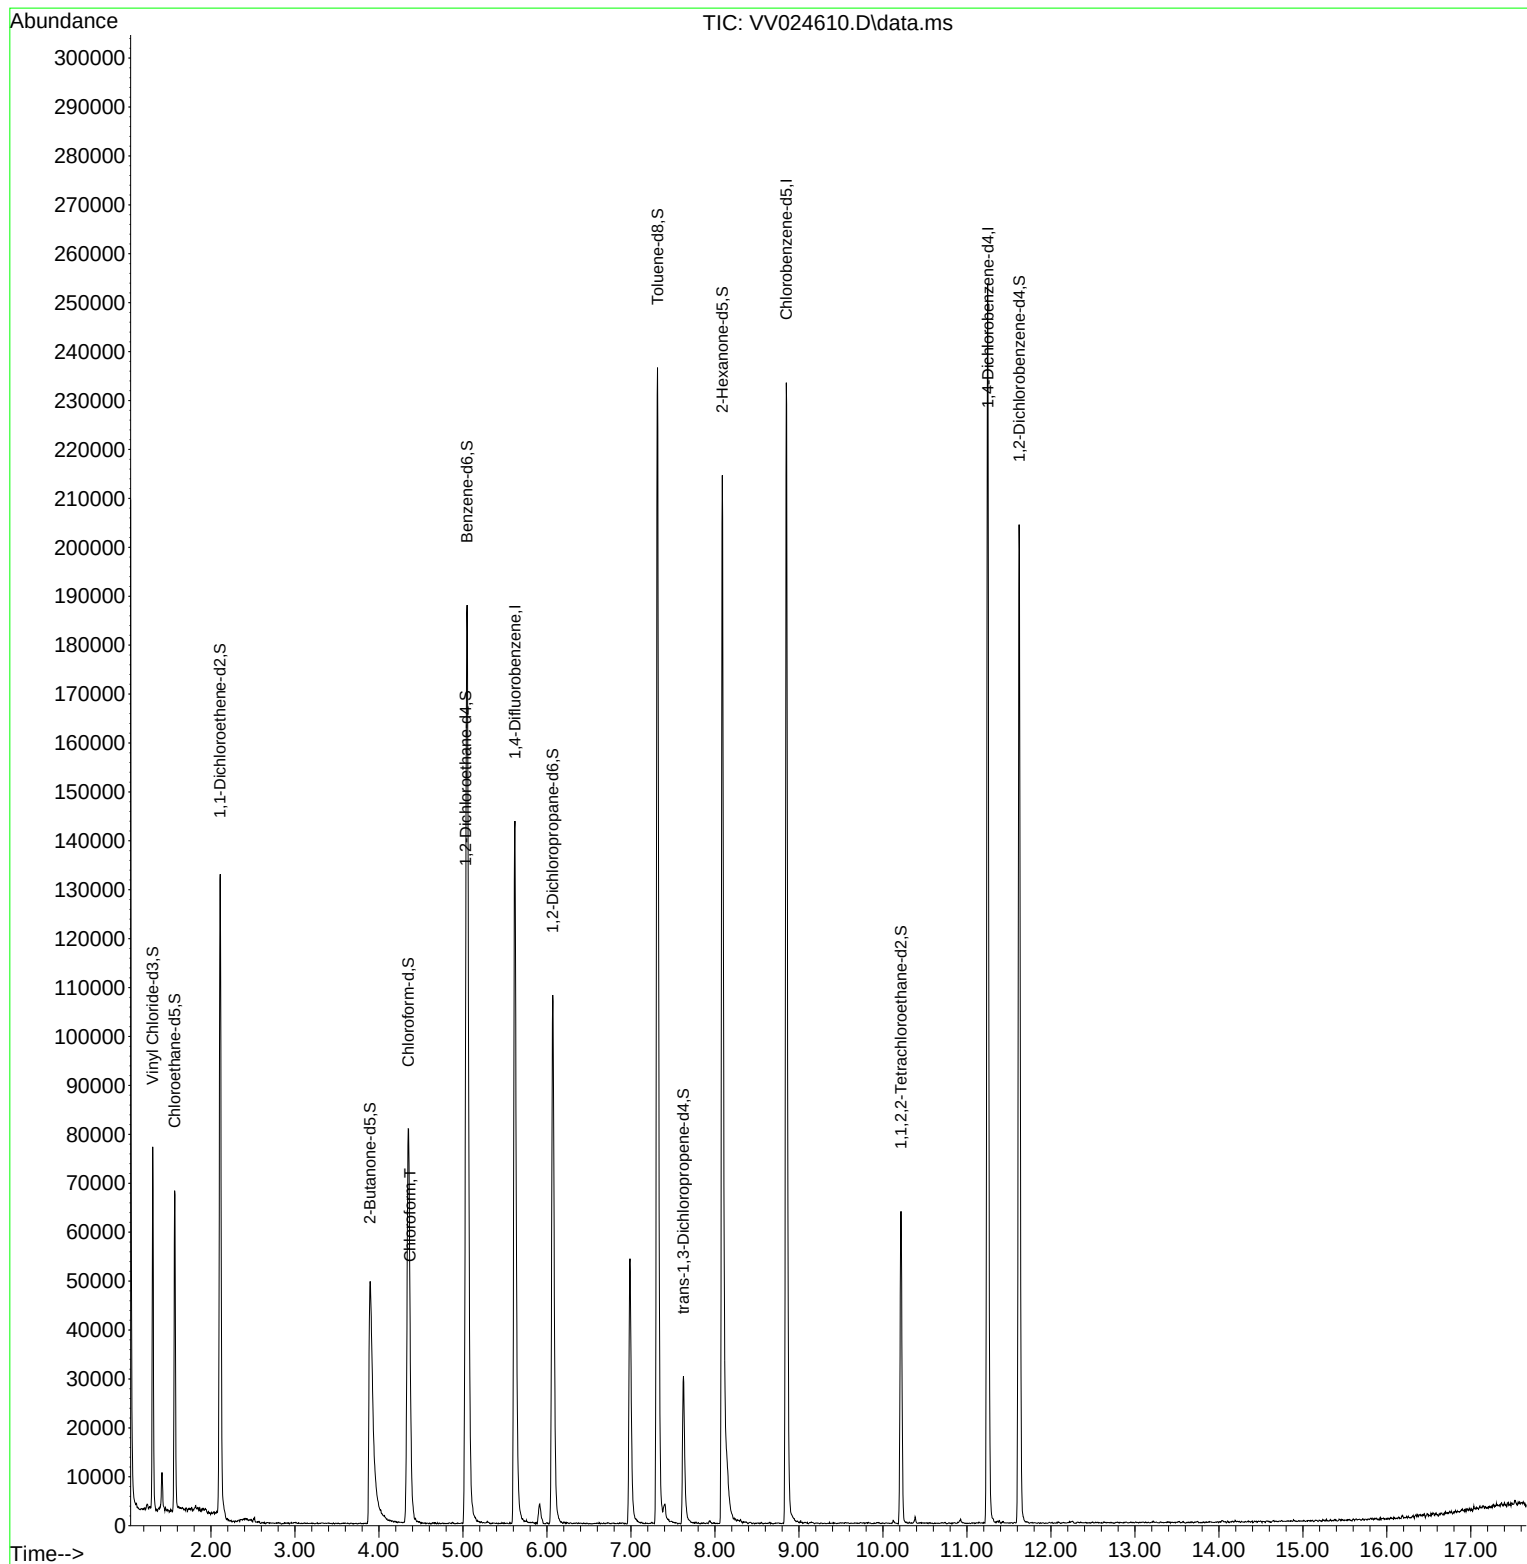

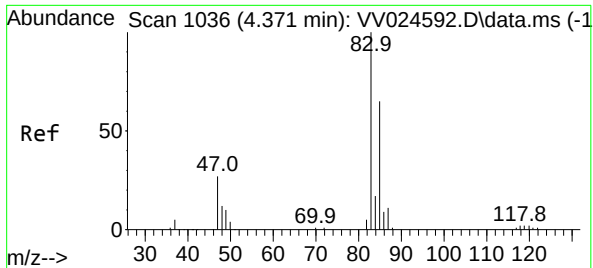

#25

Chloroform

Concen: 0.072 ug/L

RT: 4.372 min Scan# 10

Delta R.T. 0.000 min

Lab File: VV024610.D

Acq: 11 Feb 2022 17:45

Instrument :

MSVOA\_V

ClientSampleId :

GBCW2

Tgt Ion: 83 Resp: 1629

Ion Ratio Lower Upper

83 100

85 69.3 45.2 84.0

