

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
 Data File : VV024618.D
 Acq On : 11 Feb 2022 21:24
 Operator : SY/MD
 Sample : VV0211WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK303

Quant Time: Feb 12 07:09:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Feb 12 07:08:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	121620	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	120590	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	59528	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	55342	5.428	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	108.600%
7) Chloroethane-d5	1.571	69	49901	5.790	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	115.800%
11) 1,1-Dichloroethene-d2	2.111	63	89789	4.027	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.600%
20) 2-Butanone-d5	3.899	46	95736	56.569	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.140%
24) Chloroform-d	4.352	84	97048	5.409	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.200%
26) 1,2-Dichloroethane-d4	5.034	65	48220	5.923	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	118.400%
32) Benzene-d6	5.050	84	207101	6.053	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	121.000%
36) 1,2-Dichloropropane-d6	6.069	67	61895	5.816	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	116.400%
41) Toluene-d8	7.313	98	188556	5.909	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	118.200%
43) trans-1,3-Dichloroprop...	7.622	79	21537	5.011	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	100.200%
46) 2-Hexanone-d5	8.088	63	80429	53.121	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	106.240%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34154	5.390	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	56878	5.927	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	118.600%
Target Compounds						
25) Chloroform	4.381	83	3027	0.135	ug/L	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024618.D
Acq On : 11 Feb 2022 21:24
Operator : SY/MD
Sample : VV0211WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK303

Quant Time: Feb 12 07:09:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Feb 12 07:08:39 2022
Response via : Initial Calibration

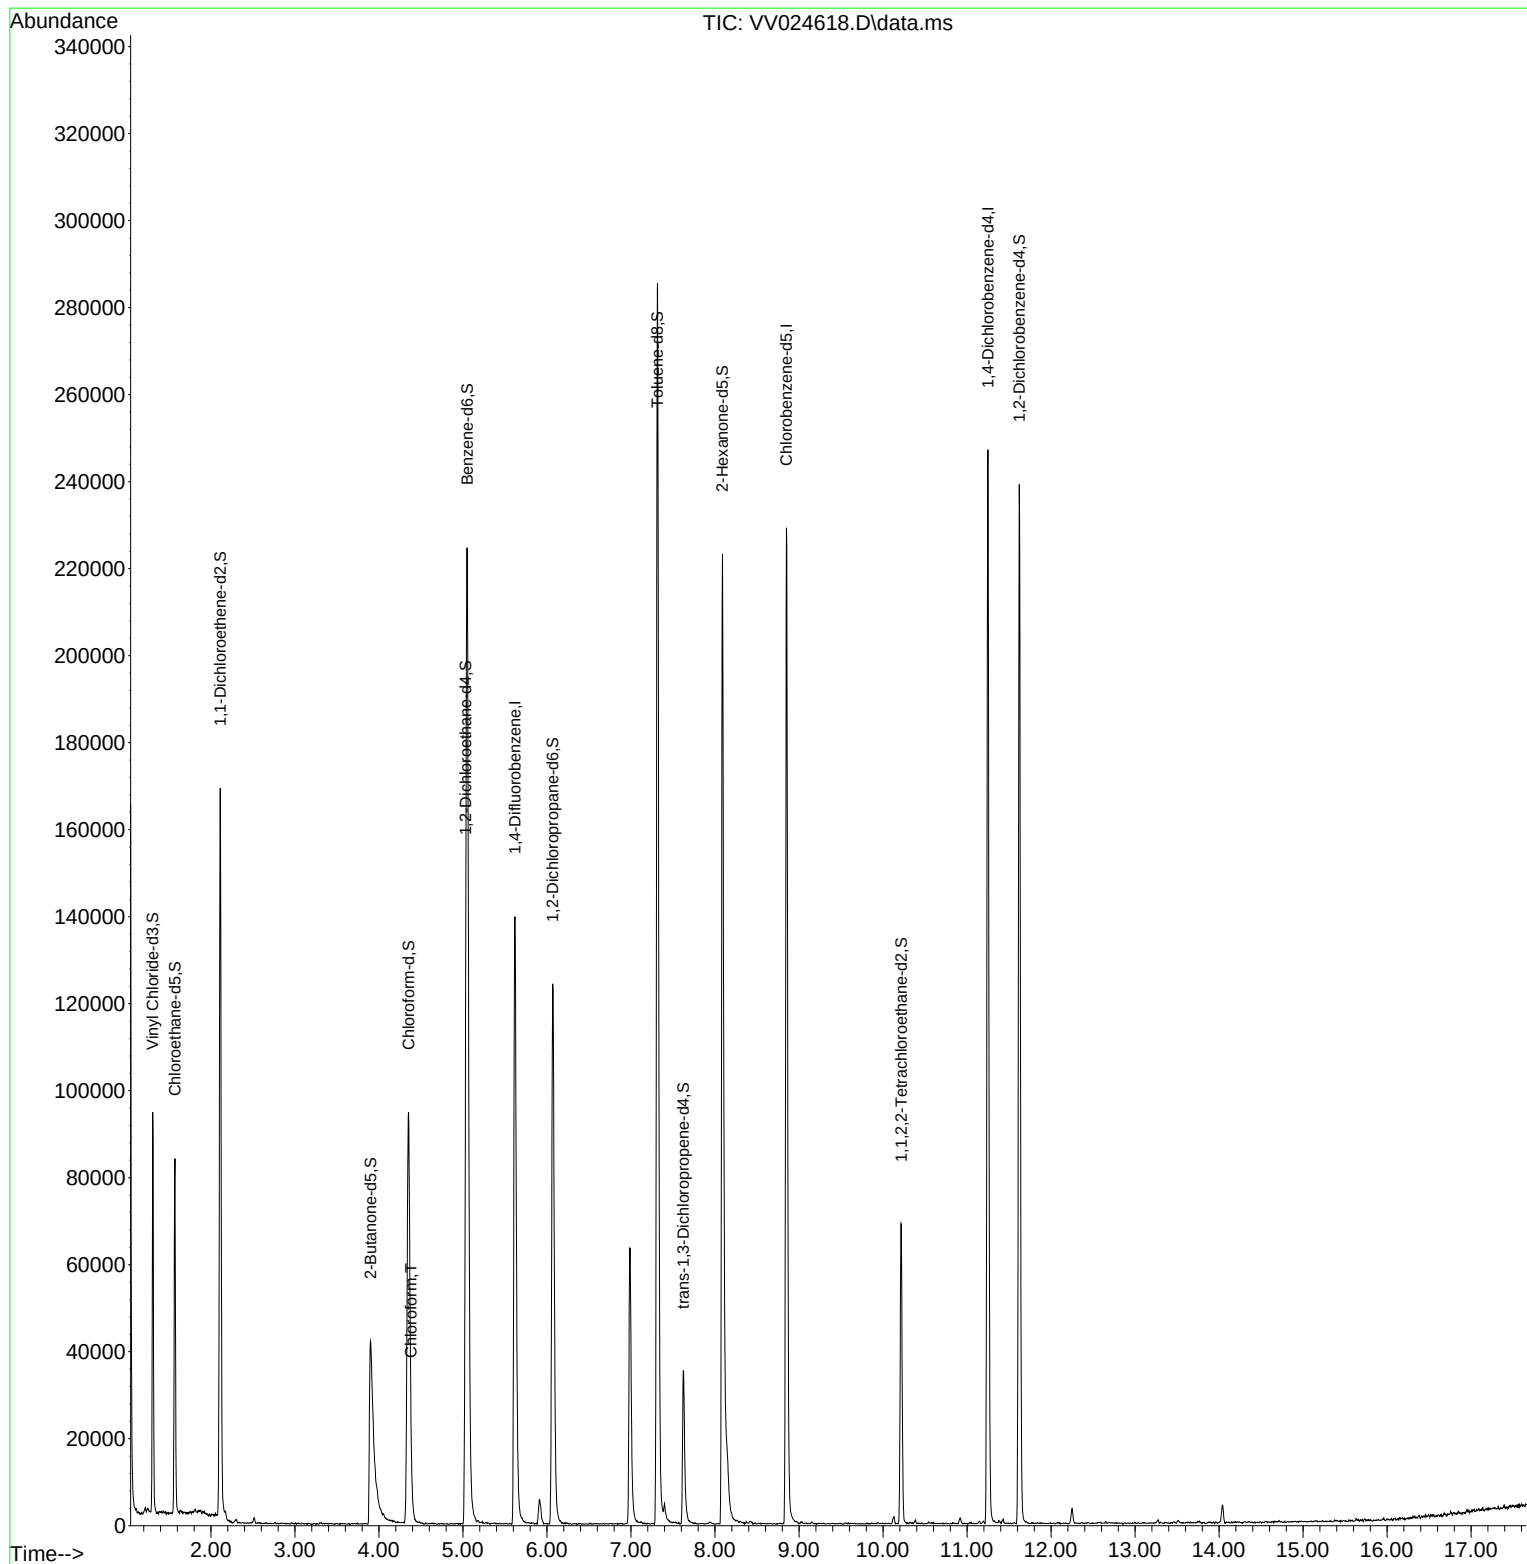

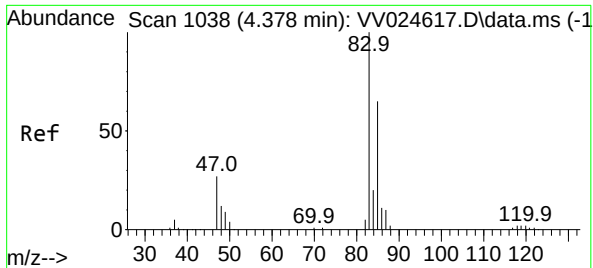

#25

Chloroform

Concen: 0.135 ug/L

RT: 4.381 min Scan# 10

Delta R.T. 0.003 min

Lab File: VV024618.D

Acq: 11 Feb 2022 21:24

Instrument :

MSVOA_V

ClientSampleId :

VBLK303

Tgt Ion: 83 Resp: 3027

Ion Ratio Lower Upper

83 100

85 73.0 45.2 84.0

