

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021122\
 Data File : VW024622.D
 Acq On : 11 Feb 2022 23:21
 Operator : SY/MD
 Sample : N1512-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA1

Quant Time: Feb 12 07:09:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Feb 12 07:08:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	117086	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	117458	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	51812	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	37640	3.835	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	76.800%	
7) Chloroethane-d5	1.571	69	35364	4.262	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	85.200%	
11) 1,1-Dichloroethene-d2	2.111	63	60156	2.802	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	56.000%#	
20) 2-Butanone-d5	3.912	46	86285	52.959	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	105.920%	
24) Chloroform-d	4.352	84	78703	4.556	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.200%	
26) 1,2-Dichloroethane-d4	5.037	65	38353	4.893	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.800%	
32) Benzene-d6	5.053	84	153184	4.596	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.000%	
36) 1,2-Dichloropropane-d6	6.069	67	48305	4.660	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	93.200%	
41) Toluene-d8	7.317	98	135223	4.350	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	87.000%	
43) trans-1,3-Dichloroprop...	7.625	79	17347	4.144	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.800%	
46) 2-Hexanone-d5	8.088	63	71146	48.243	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	96.480%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	29670	4.807	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	96.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	39457	4.724	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	94.400%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.243	50	2432	0.161	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024622.D
Acq On : 11 Feb 2022 23:21
Operator : SY/MD
Sample : N1512-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA1

Quant Time: Feb 12 07:09:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Feb 12 07:08:39 2022
Response via : Initial Calibration

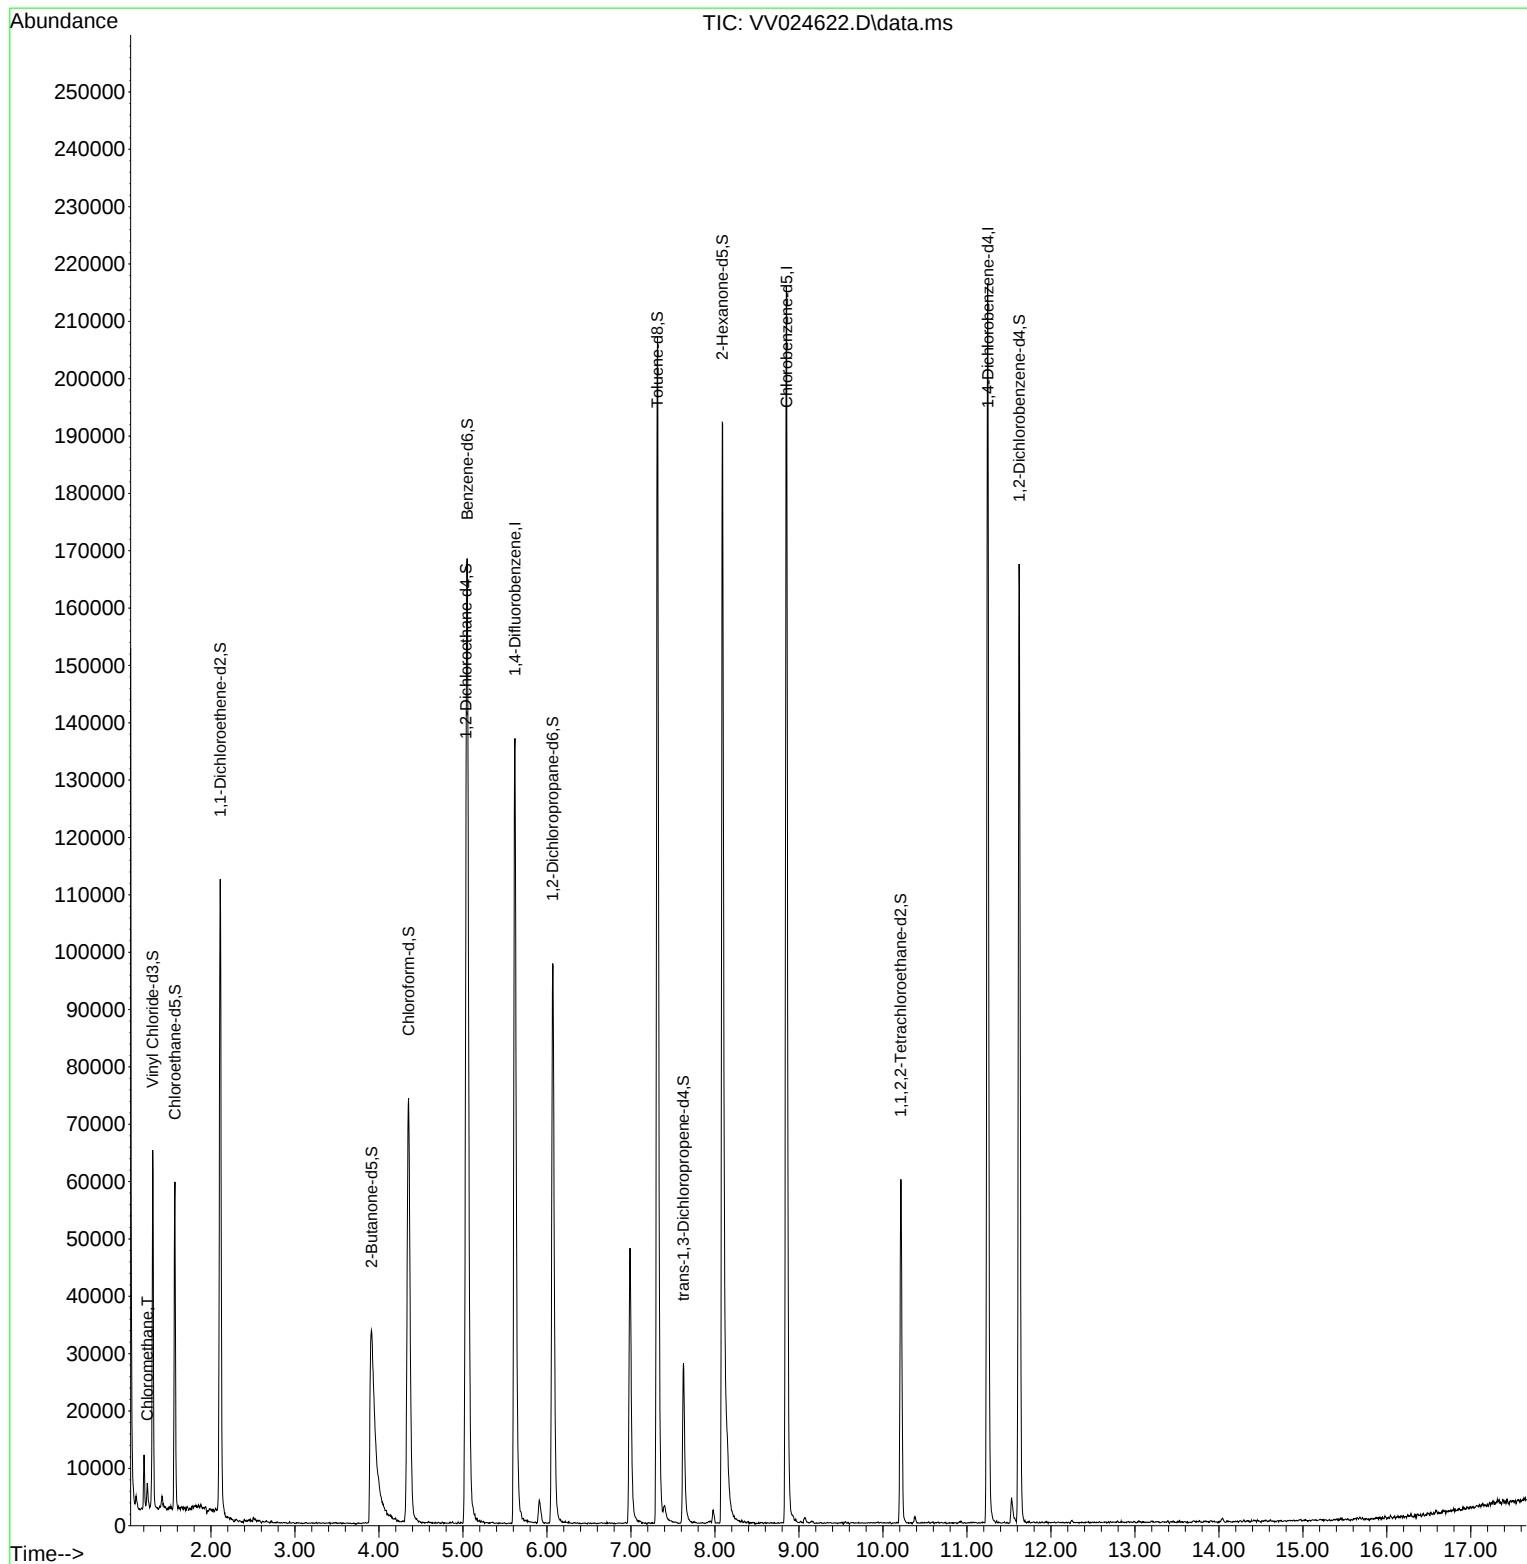

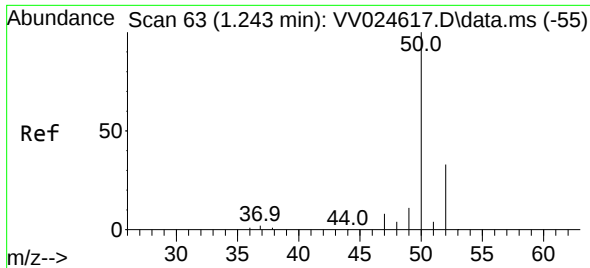

#3

Chloromethane

Concen: 0.161 ug/L

RT: 1.243 min Scan# 61

Delta R.T. 0.000 min

Lab File: VV024622.D


Acq: 11 Feb 2022 23:21

Instrument :

MSVOA_V

ClientSampleId :

C0AA1

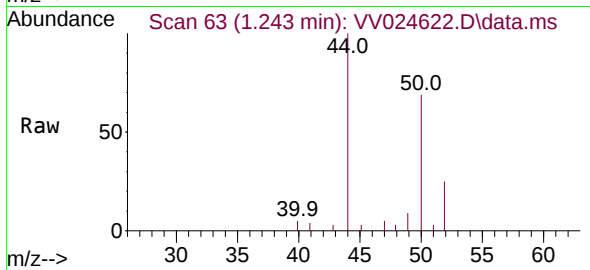

Tgt Ion: 50 Resp: 2432

Ion Ratio Lower Upper

50 100

52 36.8 22.0 41.0

