

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
 Data File : VV024593.D
 Acq On : 11 Feb 2022 10:00
 Operator : SY/MD
 Sample : VV0211WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK302

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024593.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB	73853	75308	15.53%	1.925%
2	1.571	157	165	175	rBV	64642	74148	15.29%	1.896%
3	2.111	322	333	347	rBV	131205	193500	39.90%	4.947%
4	3.896	878	888	934	rBV2	36449	142924	29.47%	3.654%
5	4.346	1010	1028	1054	rBV2	84435	213951	44.12%	5.470%
6	5.047	1230	1246	1269	rBV2	196901	484958	100.00%	12.399%
7	5.616	1410	1423	1448	rBV	139633	287309	59.24%	7.346%
8	5.908	1505	1514	1530	rVB7	4554	9895	2.04%	0.253%
9	6.066	1551	1563	1593	rBV	108864	228834	47.19%	5.851%
10	6.985	1838	1849	1868	rBV	57240	106165	21.89%	2.714%
11	7.313	1940	1951	1970	rBV	244365	425568	87.75%	10.881%
12	7.394	1971	1976	1991	rVB5	3352	7662	1.58%	0.196%
13	7.622	2035	2047	2067	rBV2	31841	58227	12.01%	1.489%
14	8.088	2182	2192	2230	rBV	198568	401526	82.80%	10.266%
15	8.850	2418	2429	2450	rBV	226984	375265	77.38%	9.595%
16	10.214	2843	2853	2870	rBV	63196	100633	20.75%	2.573%
17	11.246	3164	3174	3195	rBV	248921	385055	79.40%	9.845%
18	11.622	3279	3291	3310	rBV	215157	334841	69.05%	8.561%
19	13.506	3870	3877	3888	rBV3	3531	5469	1.13%	0.140%




Sum of corrected areas: 3911238

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024593.D
Acq On : 11 Feb 2022 10:00
Operator : SY/MD
Sample : VV0211WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK302

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

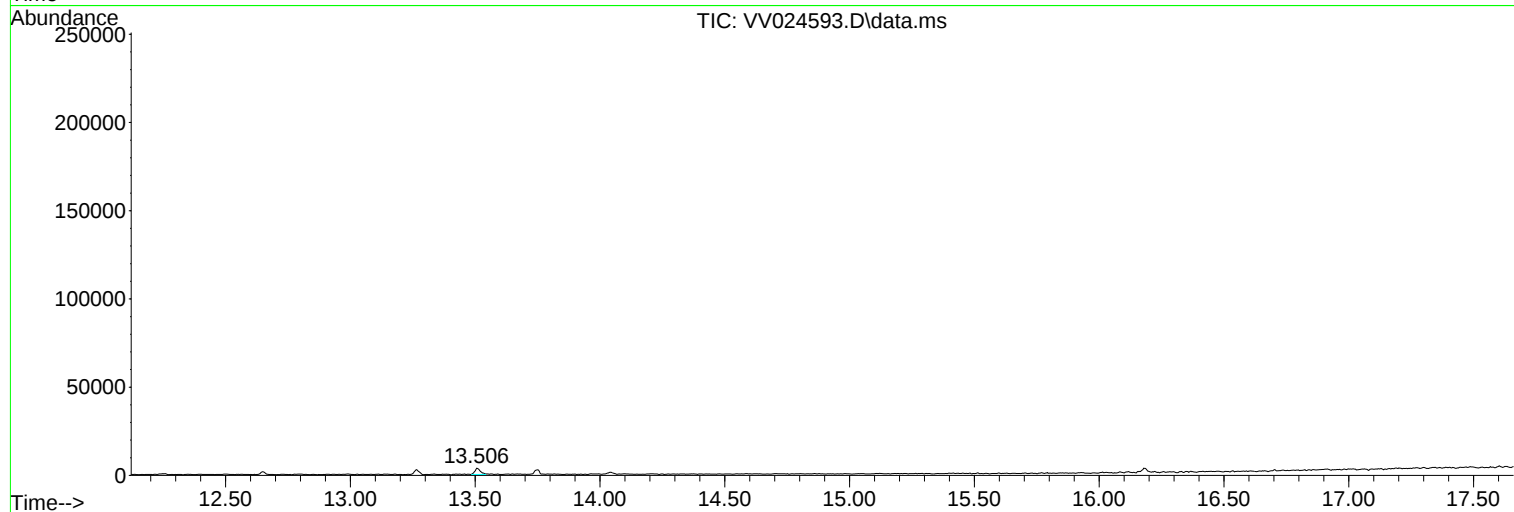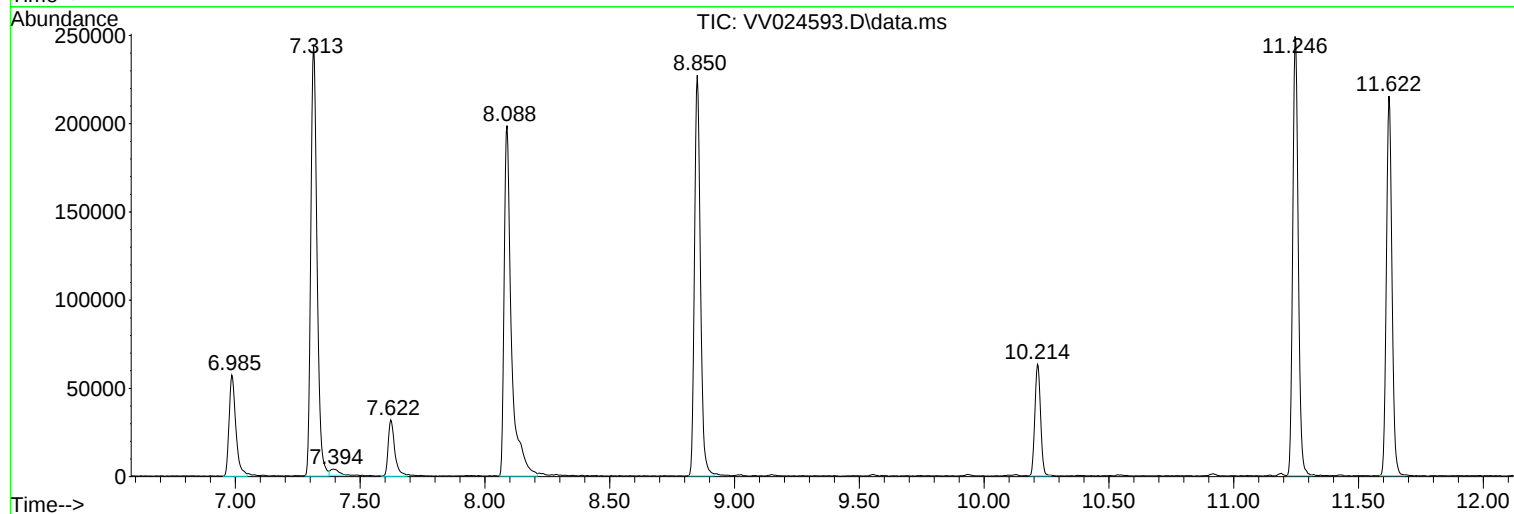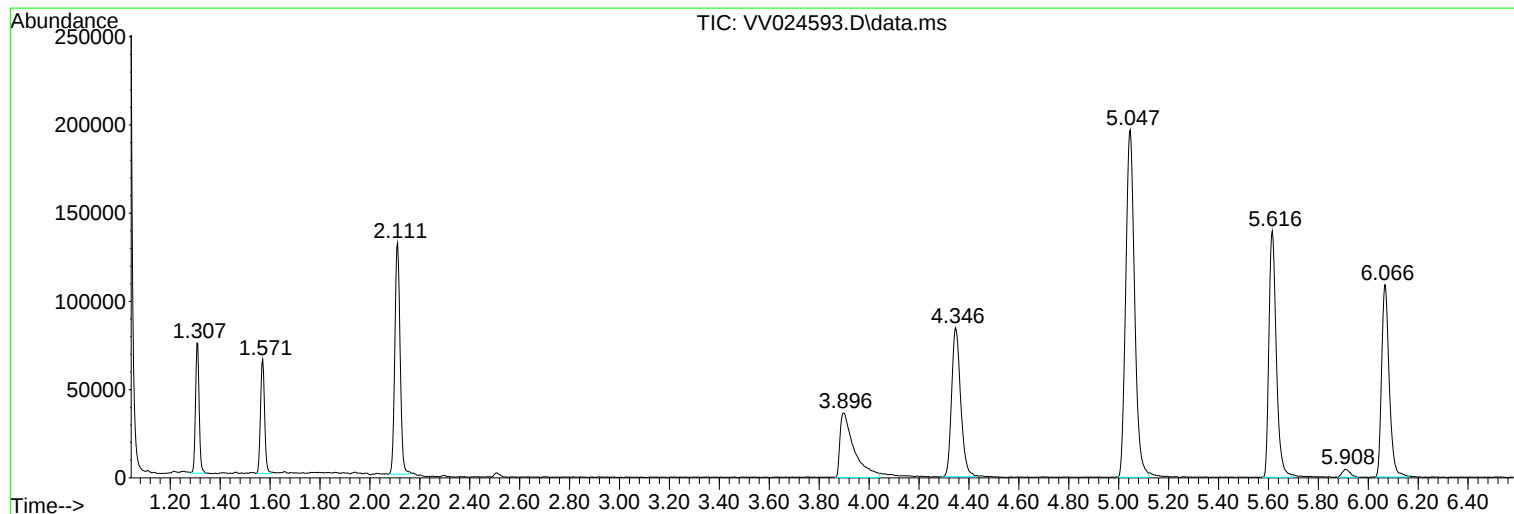

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024593.D
Acq On : 11 Feb 2022 10:00
Operator : SY/MD
Sample : VV0211WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK302

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024593.D
Acq On : 11 Feb 2022 10:00
Operator : SY/MD
Sample : VV0211WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK302

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------