

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
 Data File : VV024606.D
 Acq On : 11 Feb 2022 16:11
 Operator : SY/MD
 Sample : N1475-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M71

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024606.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	49019	50163	13.29%	1.589%
2	1.571	157	165	176	rBV	48228	54187	14.35%	1.717%
3	2.111	322	333	350	rVB	92189	136280	36.10%	4.317%
4	3.899	876	889	923	rBV	45429	155124	41.09%	4.914%
5	4.352	1012	1030	1051	rBV	63702	160564	42.53%	5.087%
6	5.050	1231	1247	1283	rBV2	144189	364338	96.52%	11.542%
7	5.619	1413	1424	1452	rBV	113432	230564	61.08%	7.304%
8	5.912	1506	1515	1531	rBV6	5670	11912	3.16%	0.377%
9	6.072	1552	1565	1591	rBV2	84642	174935	46.34%	5.542%
10	6.989	1839	1850	1873	rBV2	44130	84225	22.31%	2.668%
11	7.317	1940	1952	1970	rBV	171399	301926	79.98%	9.565%
12	7.397	1970	1977	1991	rVB2	6668	13009	3.45%	0.412%
13	7.625	2037	2048	2072	rBV2	26040	48150	12.76%	1.525%
14	7.979	2151	2158	2167	rVB5	2476	3946	1.05%	0.125%
15	8.088	2182	2192	2235	rBV	189772	377491	100.00%	11.959%
16	8.854	2418	2430	2456	rBV	186644	311348	82.48%	9.864%
17	9.146	2513	2521	2532	rBV3	3078	4869	1.29%	0.154%
18	10.217	2842	2854	2872	rVB	55962	88785	23.52%	2.813%
19	11.249	3162	3175	3196	rBV	212208	324842	86.05%	10.291%
20	11.622	3281	3291	3312	rBV	160942	259861	68.84%	8.233%




Sum of corrected areas: 3156519

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024606.D
Acq On : 11 Feb 2022 16:11
Operator : SY/MD
Sample : N1475-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

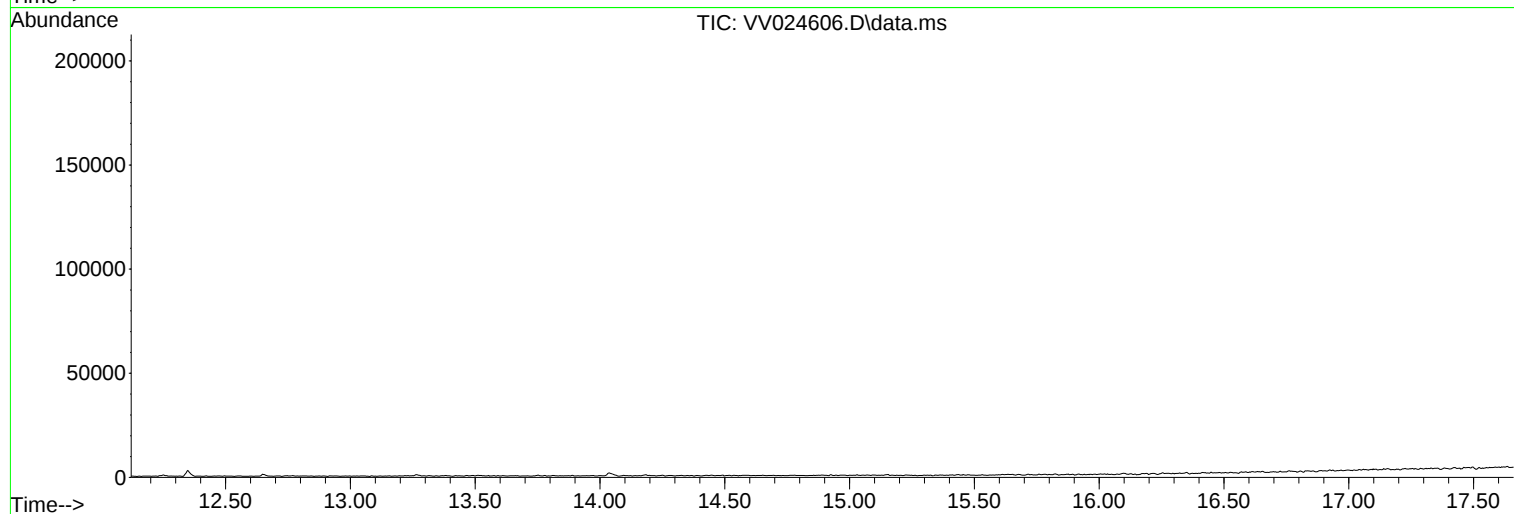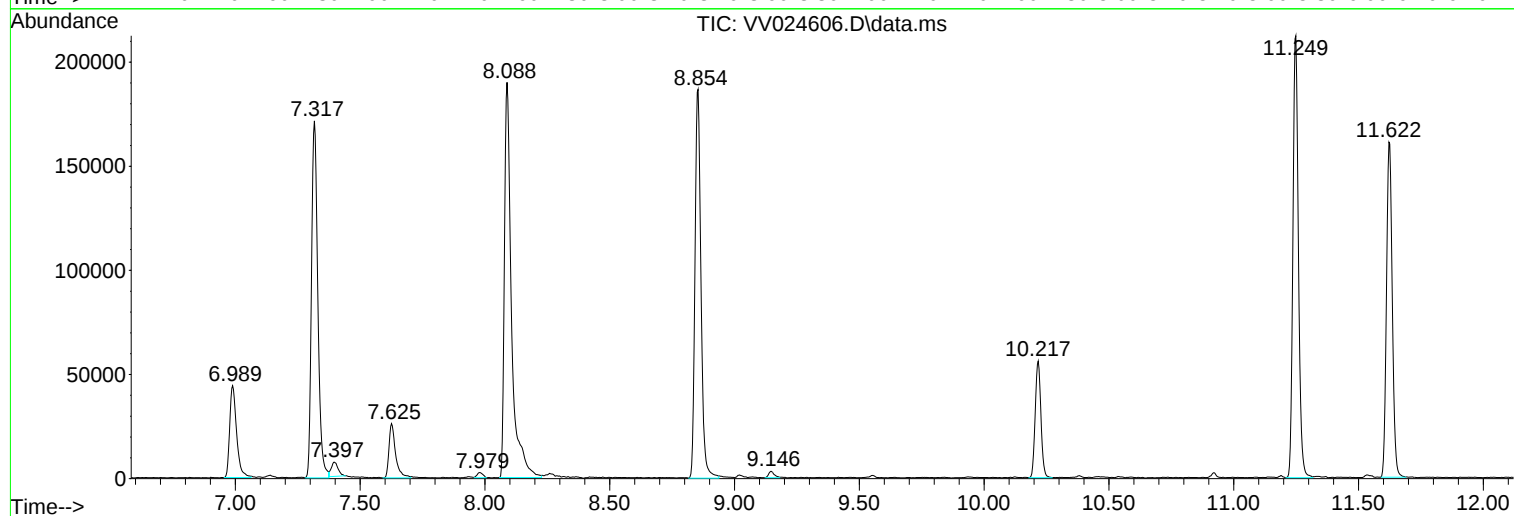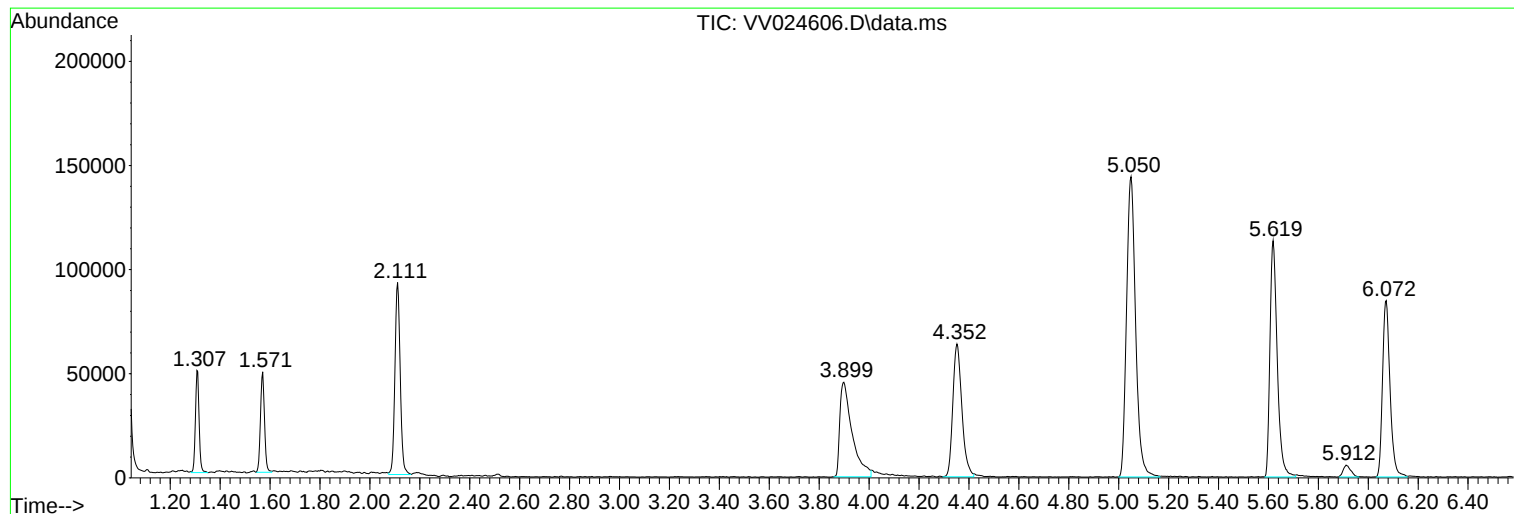

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024606.D
Acq On : 11 Feb 2022 16:11
Operator : SY/MD
Sample : N1475-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024606.D
Acq On : 11 Feb 2022 16:11
Operator : SY/MD
Sample : N1475-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
