

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
 Data File : VV024607.D
 Acq On : 11 Feb 2022 16:34
 Operator : SY/MD
 Sample : N1479-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBCT9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024607.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	73522	73964	15.47%	1.879%
2	1.420	111	118	127	rVB	8203	9358	1.96%	0.238%
3	1.571	157	165	180	rBV	66220	76361	15.97%	1.940%
4	2.111	322	333	346	rBV	131143	188400	39.39%	4.786%
5	3.896	876	888	929	rBV2	49402	170550	35.66%	4.333%
6	4.349	1014	1029	1058	rBV	82277	205806	43.03%	5.228%
7	5.050	1230	1247	1278	rBV2	193177	478262	100.00%	12.150%
8	5.619	1412	1424	1448	rBV	143008	290173	60.67%	7.372%
9	5.912	1506	1515	1531	rVB7	4090	8789	1.84%	0.223%
10	6.069	1546	1564	1594	rBV	112439	228623	47.80%	5.808%
11	6.989	1840	1850	1874	rBV	55880	104288	21.81%	2.649%
12	7.317	1940	1952	1972	rBV	238058	418462	87.50%	10.631%
13	7.397	1972	1977	1996	rVB2	4369	8523	1.78%	0.217%
14	7.625	2039	2048	2071	rBV2	31582	56398	11.79%	1.433%
15	8.088	2182	2192	2241	rBV	211177	411981	86.14%	10.466%
16	8.850	2419	2429	2455	rBV	227993	376907	78.81%	9.575%
17	10.217	2842	2854	2876	rVB	65362	103095	21.56%	2.619%
18	11.249	3164	3175	3203	rVB	255251	392297	82.03%	9.966%
19	11.535	3256	3264	3275	rBV4	2949	5333	1.12%	0.135%
20	11.622	3281	3291	3311	rVB	207446	328741	68.74%	8.351%




Sum of corrected areas: 3936311

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024607.D
Acq On : 11 Feb 2022 16:34
Operator : SY/MD
Sample : N1479-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCT9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

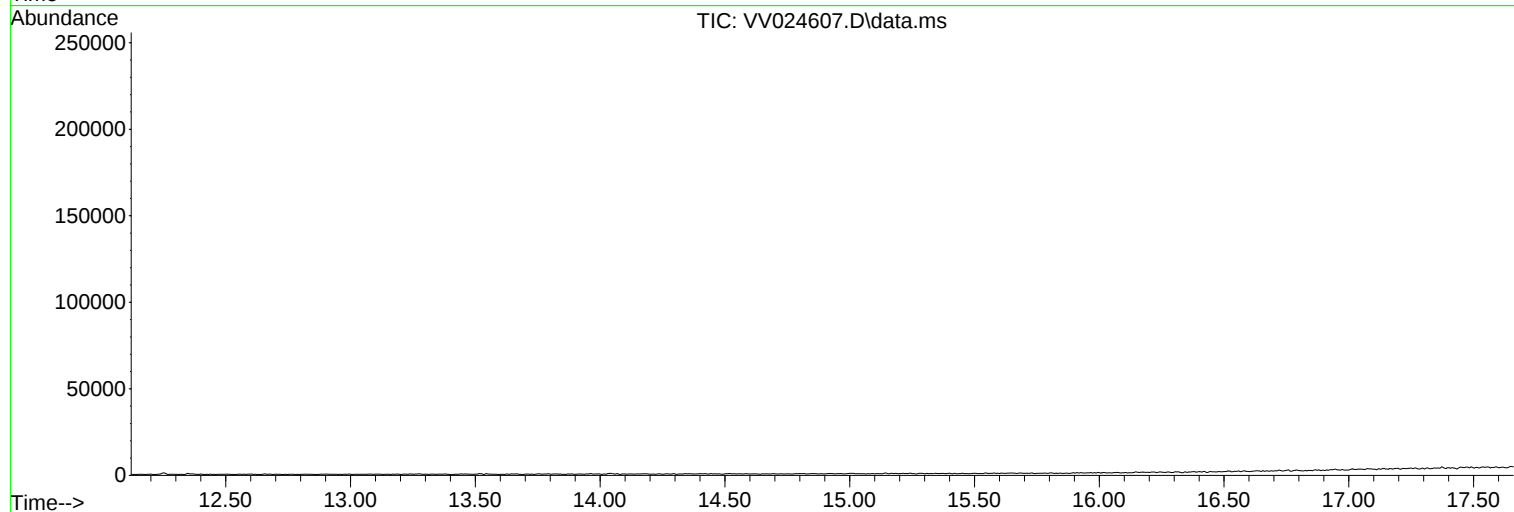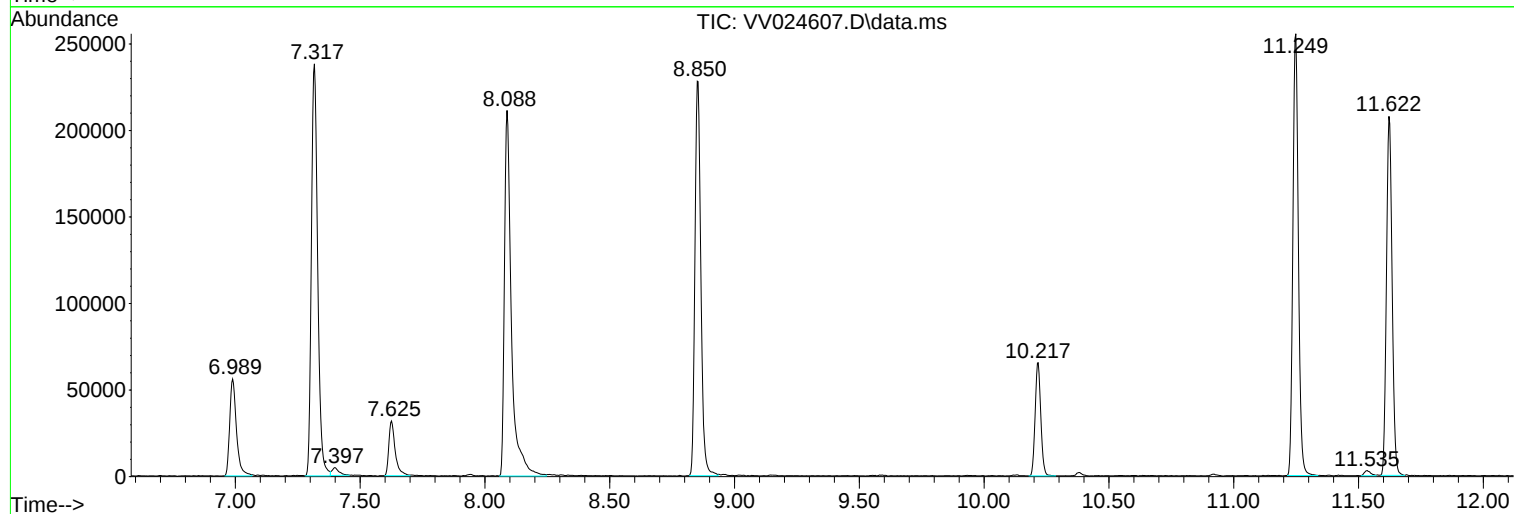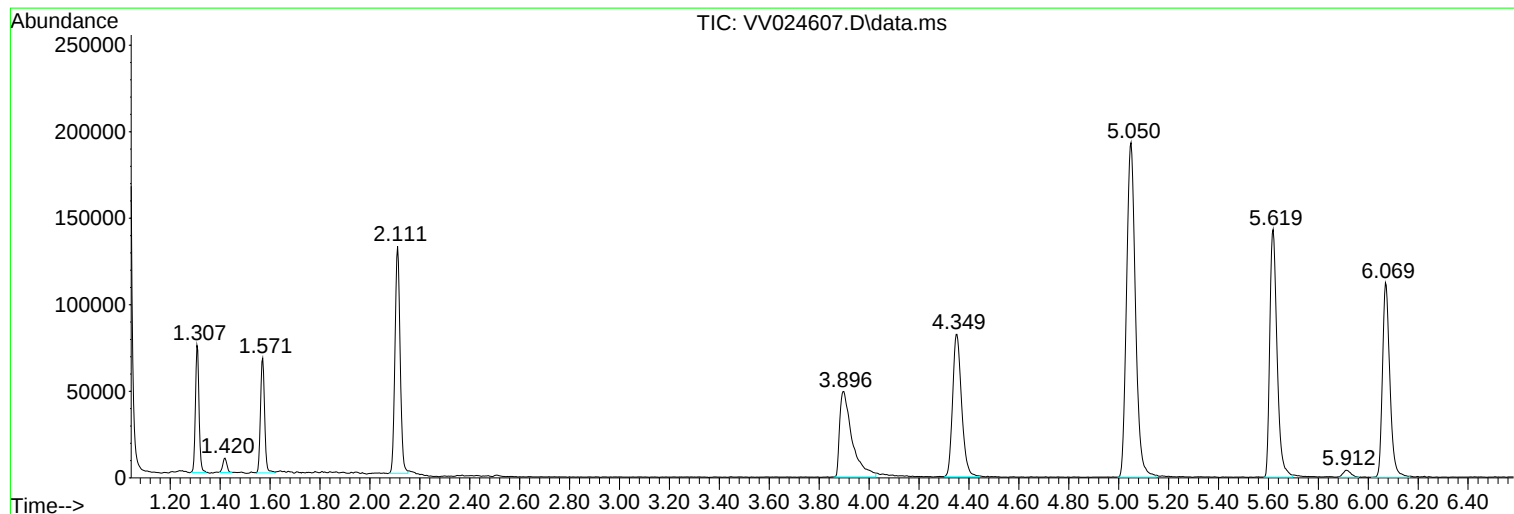

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024607.D
Acq On : 11 Feb 2022 16:34
Operator : SY/MD
Sample : N1479-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCT9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024607.D
Acq On : 11 Feb 2022 16:34
Operator : SY/MD
Sample : N1479-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCT9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
